

**TE7/TE5/TE7 Max/TE5 Max/TE9**  
**Diagnostic Ultrasound System**  
**Operator's Manual**

**[Advanced Volume]**



# Content

---

<b>Content</b> .....	<b>i</b>
Intellectual Property Statement .....	I
Preface .....	II
Safety Precautions .....	III
<b>1 Overview</b> .....	<b>1-1</b>
1.1 Measurement Preset.....	1-1
1.2 Basic Operations and Buttons.....	1-1
1.3 Measurement Menu .....	1-1
1.3.1 Measurement Location .....	1-2
1.3.2 Measurement Tool .....	1-2
1.4 Measurement, Calculation and Study .....	1-3
1.5 Measurement Caliper .....	1-4
1.6 Results Window.....	1-4
1.6.1 Results Display .....	1-4
1.6.2 Moving the Results Window .....	1-5
1.7 Cross-window Measurement.....	1-5
1.8 Report.....	1-5
1.8.1 Viewing Reports.....	1-6
1.8.2 Editing Reports .....	1-6
1.8.3 Printing Reports.....	1-7
1.8.4 Fetal Growth Curve.....	1-8
<b>2 Basic Measurement</b> .....	<b>2-1</b>
2.1 Basic Measurement Procedures .....	2-1
2.2 Basic Measurement Tools .....	2-1
2.2.1 Depth .....	2-1
2.2.2 Distance .....	2-1
2.2.3 Angle.....	2-2
2.2.4 Area & Circumference .....	2-2
2.2.5 Curve Length .....	2-3
2.2.6 Volume.....	2-4
2.2.7 Ratio (D) .....	2-4
2.2.8 Ratio (A).....	2-4
2.2.9 Smart Trace .....	2-5

2.2.10	Time .....	2-5
2.2.11	Slope.....	2-6
2.2.12	HR.....	2-6
2.2.13	Velocity .....	2-6
2.2.14	Acceleration .....	2-7
2.2.15	D Trace .....	2-7
2.2.16	D Trace (Car).....	2-10
2.2.17	PS/ED .....	2-10
2.2.18	Volume Flow .....	2-10
2.2.19	IMT.....	2-11
2.3	References .....	2-12
<b>3</b>	<b>Abdomen .....</b>	<b>3-1</b>
3.1	Abdomen Exam Preparations .....	3-1
3.2	Basic Abdomen Measurement Procedures.....	3-1
3.3	Abdomen Measurement Tools .....	3-2
3.4	Abdomen Measurement Operations .....	3-4
3.5	Abdomen Exam Report.....	3-4
<b>4</b>	<b>Obstetrics .....</b>	<b>4-1</b>
4.1	Obstetric Exam Preparations .....	4-1
4.2	Basic Measurement Procedures .....	4-1
4.3	GA .....	4-1
4.3.1	Clinical GA.....	4-1
4.3.2	Ultrasound GA .....	4-2
4.4	Obstetric Measurement Tools .....	4-3
4.5	Obstetric Measurement Operations .....	4-4
4.5.1	Measurement Tool Operations .....	4-5
4.5.2	Calculation Tool Operations.....	4-5
4.5.3	Study Tool Operations.....	4-5
4.6	Obstetric Exam Report.....	4-5
4.6.1	Fetal Biophysical Profile .....	4-6
4.6.2	Fetal Growth Curve.....	4-6
4.7	Obstetric Formula.....	4-7
4.8	References .....	4-11
<b>5</b>	<b>Cardiology .....</b>	<b>5-1</b>
5.1	Cardiac Exam Preparations .....	5-1
5.2	Basic Cardiac Measurement Procedures .....	5-1
5.3	Cardiac Measurement Tools .....	5-2
5.4	Cardiac Measurement Operations .....	5-5

5.4.1	Measurement Tool Operations .....	5-5
5.4.2	Calculation Tool Operations.....	5-7
5.4.3	Study Tool Operations.....	5-7
5.5	Cardiac Exam Report.....	5-16
5.6	References .....	5-16
<b>6</b>	<b>Vascular.....</b>	<b>6-1</b>
6.1	Vascular Exam Preparations .....	6-1
6.2	Basic Vascular Measurement Procedures .....	6-1
6.3	Vascular Measurement Tools .....	6-1
6.4	Vascular Measurement Operations.....	6-3
6.4.1	Measurement Tool Operations .....	6-3
6.4.2	Calculation Tool Operations.....	6-3
6.4.3	Study Tool Operations.....	6-4
6.5	Vascular Exam Report.....	6-5
6.6	References .....	6-5
<b>7</b>	<b>Gynecology .....</b>	<b>7-1</b>
7.1	Gynecology Exam Preparations.....	7-1
7.2	Basic Gynecology Measurement Procedures.....	7-1
7.3	Gynecology Measurement Tools.....	7-1
7.4	Gynecology Measurement Operations.....	7-2
7.4.1	Measurement Tool Operations .....	7-2
7.4.2	Calculation Tool Operations.....	7-2
7.4.3	Study Tool Operations.....	7-3
7.5	Gynecology Exam Report .....	7-4
7.6	References .....	7-4
<b>8</b>	<b>Urology .....</b>	<b>8-1</b>
8.1	Urology Exam Preparations .....	8-1
8.2	Basic Urology Measurement Procedures .....	8-1
8.3	Urology Measurement Tools .....	8-1
8.4	Urology Measurement Operations .....	8-2
8.4.1	Measurement Tool Operations .....	8-3
8.4.2	Calculation Tool Operations.....	8-3
8.4.3	Study Tool Operations.....	8-4
8.5	Urology Exam Report.....	8-5
8.6	References .....	8-5
<b>9</b>	<b>Small Parts .....</b>	<b>9-1</b>
9.1	Small Parts Exam Preparations .....	9-1
9.2	Basic Small Parts Measurement Procedures .....	9-1

9.3	Small Parts Measurement Tools.....	9-1
9.4	Small Parts Measurement Operations .....	9-3
9.4.1	Measurement Tool Operations .....	9-3
9.4.2	Calculation Tool Operations.....	9-3
9.4.3	Study Tool Operations.....	9-3
9.5	Small Parts Exam Report.....	9-4
9.6	References .....	9-4
<b>10</b>	<b>Pediatrics.....</b>	<b>10-1</b>
10.1	Pediatrics Exam Preparations.....	10-1
10.2	Basic Pediatrics Measurement Procedures .....	10-1
10.3	Pediatrics Measurement Tools .....	10-2
10.4	HIP Measurement Operations.....	10-4
10.5	Pediatrics Exam Report .....	10-4
10.6	References .....	10-4
<b>11</b>	<b>Emergency&amp;Critical.....</b>	<b>11-1</b>
11.1	Basic Measurement Procedures .....	11-1
11.2	EM Measurement Tools.....	11-1
11.3	EM Exam Report.....	11-1
<b>12</b>	<b>Nerve.....</b>	<b>12-1</b>
12.1	Basic Measurement Procedures .....	12-1
12.2	Nerve Measurement Tools .....	12-1
12.3	Nerve Exam Report.....	12-1

© 2014-2021 Shenzhen Mindray Bio-medical Electronics Co., Ltd. All Rights Reserved.

The issue date of this Operator's Manual is 2021-07.

## Intellectual Property Statement

SHENZHEN MINDRAY BIO-MEDICAL ELECTRONICS CO., LTD. (hereinafter referred to as Mindray) owns the intellectual property rights to this Mindray product and this manual. This manual may refer to information protected by copyright or patents and does not convey any license under the patent rights or copyright of Mindray or of others.

Mindray intends to maintain the contents of this manual as confidential information. Disclosure of the information in this manual in any manner whatsoever without the written permission of Mindray is strictly forbidden.

Release, amendment, reproduction, distribution, rental, adaptation, translation or any other derivative work of this manual in any manner whatsoever without the written permission of Mindray is strictly forbidden.

### **IMPORTANT!**

1. No part of this manual may be copied or reprinted, in whole or in part, without written permission.
2. The contents of this manual are subject to change without prior notice and without our legal obligation.

# Preface

This manual details the procedures for operating this system . Carefully read and understand the manual before using the system to ensure its safe and correct operation.

**NOTE:** When operating the system, refer to the following manuals:

- Operator's Manual (Basic Volume)
- Acoustic output data

Depending on the software version, the preset settings, optional configuration and the actual interfaces may appear differently from those shown in this manual.

**NOTE:** The functions described in this manual are not provided for all systems sold in all regions. The functions available depend on the specific system purchased.

All the menus and screenshots in this manual take the system in full configuration as an example.




# Safety Precautions

## 1. Meanings of Signal Words

In this manual, the signal words **⚠️ Danger**, **⚠️ WARNING**, **⚠️ CAUTION** and **NOTE** are used regarding safety and other important instructions. The signal words and their meanings are defined as follows. Please understand their meanings clearly before reading this manual.

Signal word	Meaning
<b>⚠️ Danger</b>	Indicates an imminently hazardous situation that, if not avoided, will result in death or serious injury.
<b>⚠️ WARNING</b>	Indicates a potentially hazardous situation that, if not avoided, could result in death or serious injury.
<b>⚠️ CAUTION</b>	Indicates a potentially hazardous situation that, if not avoided, may result in minor or moderate injury.
<b>NOTE</b>	Indicates a potentially hazardous situation that, if not avoided, may result in property damage.

## 2. Meaning of Safety Symbols

Symbol	Description
	General warning, caution, risk of danger.

## 3. Safety Precautions

Please observe the following precautions to ensure patient and operator safety when using this system.

<b>⚠️ CAUTION:</b>	<ol style="list-style-type: none"> <li>1. <b>Select the proper patient image and measurement tools. Only qualified professionals can decide the appropriate measurements and results.</b></li> <li>2. <b>Confine measurement calipers to the actual Region of Interest (ROI). Measurements that extend beyond the ROI will be incorrect.</b></li> <li>3. <b>Before examining a new patient, it is necessary to tap [End] to end the current scan and delete the patient information and data. Failure to do so will result in new patient data being combined with the previous patient's data.</b></li> <li>4. <b>When the system is turned OFF or [End] is tapped, all unsaved data are lost.</b></li> <li>5. <b>Changing modes during a measurement will delete the Basic Measurement data.</b></li> <li>6. <b>Tap [Freeze] to unfreeze the image during a measurement will clear the Basic Measurement data.</b></li> <li>7. <b>Tap [Clear All] will clear the measurement caliper and all data in the result window, such as comments and body marks.</b></li> </ol>
--------------------	---

- 8. In dual-B imaging mode, the measurement results of the merged image can be inaccurate. Therefore, the results are provided for reference only, not for confirming diagnoses.**
- 9. Ensure that measurement data correctly corresponds to the fetus during the Obstetric Measurement.**
- 10. Fully understand the functionality of this system by referring to the *Operator's Manual - Basic Volume*.**
- 11. When the result of auto trace does not match the image exactly, perform the measurement manually.**

# 1 Overview

---

## 1.1 Measurement Preset

Before measuring, preset the following parameters:

- Measurement Parameters Preset
- Obstetric Preset
- Basic Measurement Preset
- Advanced Measurement Preset
- Report Preset

For detailed information about Measurement Preset, see the the Operator's Manual [Basic Volume] for details.

## 1.2 Basic Operations and Buttons



### Basic Measurement Procedures

1. Tap [End] to end the last exam.
2. Tap [Patient] and enter the patient information,  
This includes patient ID, name, height, weight, etc. Enter manually for a new patient or load from iStation or Worklist for an anonymous patient.  
The patient information entered is used for measurement data storage, analysis and exam report. For more details, see “Exam Preparation → Patient Information” in the Operator's Manual [Basic Volume].
3. Tap [Probe] and select a proper exam mode.  
For more details, see “Exam Preparation” in the Operator's Manual [Basic Volume].
4. Tap [Measure] to start measurement.
5. Select an item from the measurement menu to start.  
For basic and advanced measurement items (tools), see chapter “2 Basic Measurement” of the specified advanced measurements for details.
6. Tap [Report] to view the exam report.  
For report editing and browsing, see “1.8 Report.”


## 1.3 Measurement Menu

The Basic and Advanced measurement menus are different. For more information on the measurement menu, see “2 Basic Measurement” and the specified advanced measurement chapters.

The measurement menus are shown in the following figures:

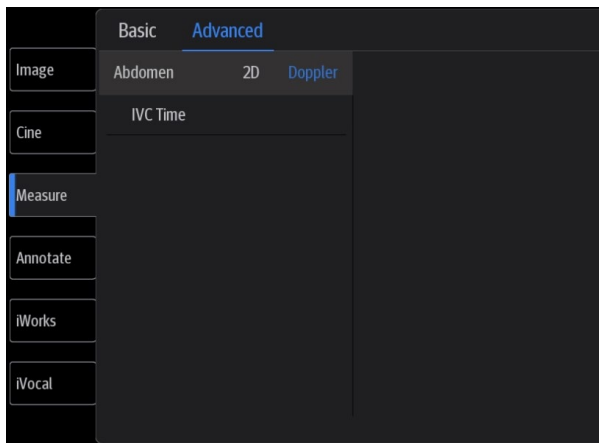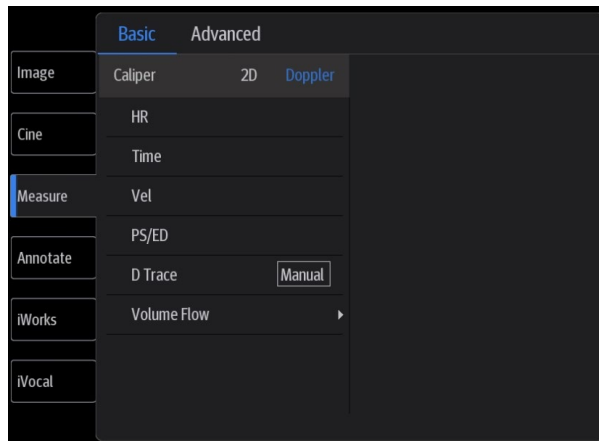

### 1.3.1 Measurement Location

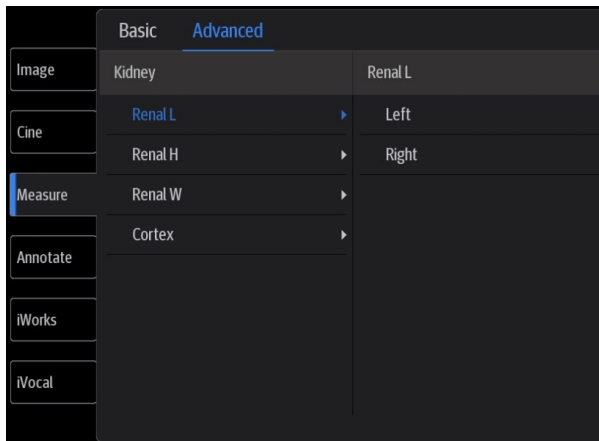

The location widgets are used to select the measurement locations.

- Side (Left/Right): belongs to items (e.g., kidney) that contain measurements of left/right side parameters respectively.
- Location (Prox./Mid./Dist.): belongs to items (e.g., vascular) that contain measurements of Proximal, Middle or Distal parameters.

**Tip:** The location widgets are applicable only in the advanced measurements.

### 1.3.2 Measurement Tool

There are two types of measurement tools.

- Basic tools: the measurement tools for Basic Measurements which are general and have no specific clinical definitions. Examples include “Distance” and “Area”.
- Advanced tools: the measurement tools for Advanced Measurement. These items are classified and combined in clinical advanced packages according to the exam mode. For example, HC (head circumference) in the Obstetric measurements is one of the advanced tools.

### To Activate the Measurement Tool


The procedure is as follows:

1. Select the tool: Tap the screen to select the item and tap again to confirm.  
For 2D+M and 2D+Doppler combined imaging modes, the measurement items will be classified according to the imaging modes.  
Tap the imaging mode from the measurement menu, then select and perform the corresponding measurement item.
2. After finishing the measurement, perform other necessary operations.

### Select Measurement Method Online

Some measurement tools have multiple methods to select.

1. Select item in the menu.
2. Tap the box on the right side of the item to select the method, as shown in the following figure.

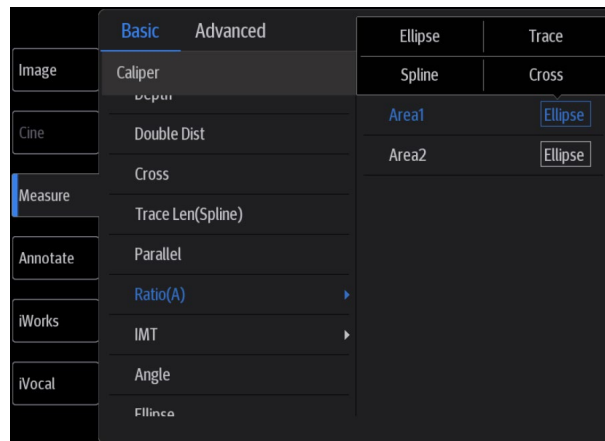


### Other Features

Features	Descriptions
Current measurement tool/item	Highlighted in blue.
Measured item	A performed advanced item/tool is marked with a “√.” (If all items in a submenu (extended menu) of a study are already performed, this study will be marked as measured.) NOTE: Tap on “√” ahead of the measured item/tool, and tap [Delete] from the menu popped up, the measure caliper and results in the result window and report will be cleared.

## 1.4 Measurement, Calculation and Study


There are three kinds of measurement items.

## Measurement

Results of measurements are directly obtained via the measurement tools, which are indicated by “” in the preset screen ([Presets] -> [Measure]).

For example, “Distance” in the 2D general measurement or “HC” in the OB measurement.


## Calculation

Results of calculations are automatically derived by the system using other measured or calculated values as parameters, they are indicated by “” in the preset screen ([Presets] -> [Measure]).

For example, EFW (Estimated Fetal Weight) in the OB measurement.

If all measurements related to a calculation tool are completed, the system will automatically calculate the result. If some measurement tools are performed again, the system will automatically update the calculation result using the latest measurement results.

## Study

A group of measurements and/or calculations for a specific clinical advanced, which are indicated by “” in the preset screen ([Presets] -> [Measure]).

For example, AFI in the OB measurement.

# 1.5 Measurement Caliper

A measurement caliper is a graphic consisting of several points and a straight line or curve drawn on the ultrasound image.

## Fixed/Active End


The ends of calipers can be active or fixed. The active end is called a Cursor.

## Caliper Color

An active caliper appears green, while a fixed one appears white in the system default preset.

## Caliper End Symbols

8 symbols are used as caliper ends, as shown in the figure below.



These symbols display in calipers as well as in the results window to identify different measurements.

**NOTE:** You can preset the cursor type in [Setup] -> [System] -> [Measure].

# 1.6 Results Window

The measurement window displays the conducted measurement's result and the engaging measurement in real time.

## 1.6.1 Results Display

The latest results are displayed in the results window in time sequence.

When viewing the results:

- If the results window is full, the oldest value will be replaced according to the “first in, first out” rule.

A maximum of 8 results can be displayed in the results window.

- To identify the measurement results, symbols or numbers are used in the numerical results window.
- To delete the last measurement result, tap [Clear Item], the measurement result, the corresponding caliper and data will be cleared.

The results displayed can be the following:

- No result displays when a measurement item/tool is activated but without fixing the start point.
- The result displays as digits when the value obtained is within the clinical range.
- The result displays as “?” when it is out of the ultrasonic range.

## 1.6.2 Moving the Results Window

To move the results window,

1. Tap on the results window title and the border of the result window will change to white.
2. Drag the results window to the desired position and release the cursor.

## 1.7 Cross-window Measurement

For linear probing, cross-window measurement is available in dual-B mode when the left and right windows are imaging with the same probe, depth and invert mode.

## 1.8 Report

The report records measurement results, which are automatically saved by the system after each measurement.

- Tap [Report] to enter the report dialog box.
- The default report of the current exam appears.
- After viewing, tap [Cancel] or [Done] to exit the report page.

## 1.8.1 Viewing Reports

Items on the report page are described as follows:

The screenshot shows a medical report interface with the following elements:

- Navigation tabs: Patient, Review, Report (selected).
- Header information: Name (dropdown), ID (20210315-170133-2BD6), Image(0) button, and Comments button.
- Measurement options: Measurement (selected) and Checklist.
- Table headers: Formula, Value, GA, 1, 2, 3, Method.
- Section: 2D Measurements.
- Measurement row:  GS, Hansmann (dropdown), 4.15cm, 9w1d, 4.17, 4.14, [empty], Avg (dropdown).

- Each measurement contains the three latest values and a final value..
- The report only displays results of tools that are displayed in the report template by default and are completed, as shown in the figure above.
- Drag the page downward if the report has more than one page.

## 1.8.2 Editing Reports

### Editing Measurement Data

**⚠ CAUTION:** Input appropriate data when editing the measurement values, otherwise misdiagnosis may occur.

- The measurement values in the text boxes are editable. Move the cursor to the text box and tap on the screen to type on the popped-up keyboard.
- The modified value(s) is/are underlined.
- The final value displays in the [Value] column. Select an option ([Last], [Avg.], [Max.] or [Min.]) from [Method] to determine the method in which the final value is calculated.
- For result values used to calculate GA (Gestational Age) and SD (Standard Deviation), the formula used in this calculation can be selected from [Formula]. The GA and SD values will update with the formula change.

**NOTE:**

1. Only measurement values are editable while calculation values are not.
2. After a measurement value is modified, the corresponding calculation value will be updated automatically.




## Entering Ultrasound Remarks

In the [Comments] box, enter the corresponding information.

## Selecting Images

Images saved for the current exam can be added to the report.

1. Tap [Image] on the report page to bring up the following dialog box.

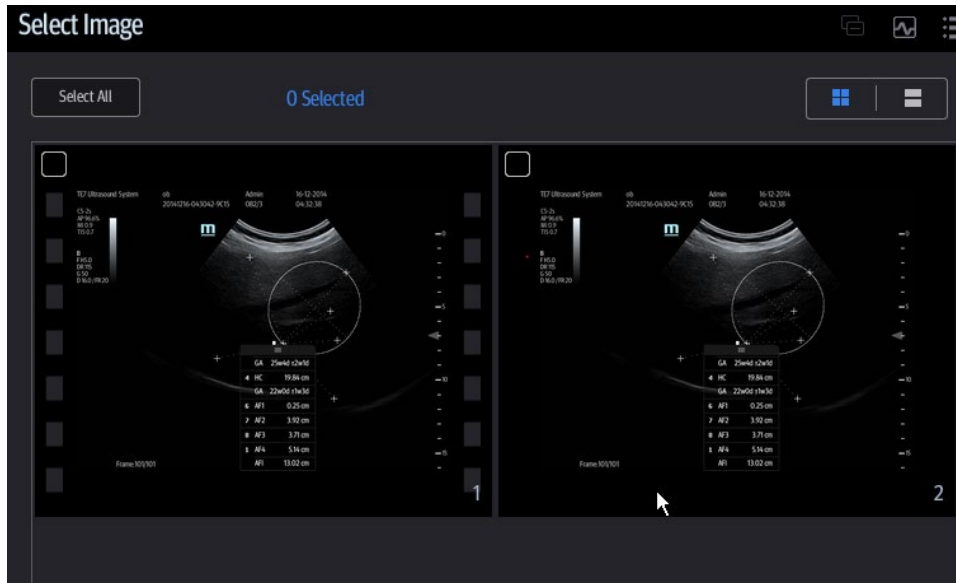

2. Select the image by tap on the check box at the upper left corner of the image.
3. Tap [Done] to confirm.

## Analyzing Report Data

You can preset and edit anatomy information in the OB report.

1. Tap [Checklist].
2. Select or enter anatomy descriptions.

**Tip:** Descriptions of [Fetus Score] can only be selected from the drop-down list.

Drag the page downward to see more measurement values.

3. Tap [Done] to confirm. Analysis information displays after the measurement values in the report.

## Signature

Fill in the signature after completing the report.

1. Tap [Signature]. Draw the signature information on the touch screen. Tap [OK] to save the information.
2. Print or preview the report to view the signature information.

## 1.8.3 Printing Reports

Tap [Preview] on the report page to preview. On the preview page, you can:

**Print report:** Tap [Print].

**Select ultrasound image layout:** Select from the drag-down list. Options:  
1/Row, 2/Row, 3/Row, 4/Row,

- Comments/  
Ultrasound  
Image/ Checklist** Tap the checkbox to select if the comments/ ultrasound image/ checklist are included when printing the report.
- Export report:** Tap [Export] and select driver, path and file type, input file name. You can also create, delete or rename the folder.
- Print setting** Tap [Print Setting], and tick the checkbox before “Show all fetus data in one report”, and the report chooses and prints the multi-fetus data simultaneously.
- Save image:** Save the report as image for the non-anonymous patient (patient with ID). You can view the saved images by tapping [Review] or [iStation] from the main screen.
- Exit the preview:** Tap [Back] to return to the report page.

## 1.8.4 Fetal Growth Curve

If [Obstetric] in the [Patient Info] is selected in the report template (see “4.6.2 Fetal Growth Curve”), you can view the fetal growth curve by touching [OB Graph] on the touch screen. See “4.6.2 Fetal Growth Curve” for details.

# 2 Basic Measurement

---

There are 2D (B/Color/Power), M and Doppler (PW/CW) basic measurement tools.

## 2.1 Basic Measurement Procedures

1. Start the exam.
2. Select the imaging mode, then scan the image.
3. Tap [Measure] to enter the measurement menu. Item available in current exam mode are displayed.
4. Select an item from the basic measurement menu to start the measurement.

The following icon appears on the screen:



Operations for the icon as follows:

- Drag and hold the hand icon to move the cursor to the desired point.
- Tap the arrows around the hand icon to fine-tune the cursor position.

## 2.2 Basic Measurement Tools

### 2.2.1 Depth

**Function:** On 2D image,

- Sectoral surface probe: the depth is the distance from the center of the sector to the cursor.
- Convex array or linear array probe: the depth is the distance from the transducer surface to the measuring cursor in the direction of the ultrasonic wave.

1. Tap [Depth] in the measurement menu.
2. Move the cursor to the desired point.
3. Tap the hand icon to set the measurement point and the result displays in the results window.

### 2.2.2 Distance

**Function:** On 2D/M image, measures the distance between two points on the image.

■ On 2D image

1. Tap [Distance] in the measurement menu.
2. Move the cursor to the starting point.
3. Tap the hand icon to set the starting point.
4. Move the cursor to the end point. Then  
Tap [Clear Item]/[Clear All] to cancel setting the starting point. Or

Tap [Update] to switch between the fixed end and the active end of the caliper. Or,  
Tap the arrows around the hand icon to fine-tune the cursor position.

5. Tap the hand icon to set the end point.

■ On M image

1. Tap [Distance] in the measurement menu.
2. Move the cursor to the starting point and tap the hand icon.
3. Move the cursor to the end point. The cursor can then only be moved in a vertical direction.  
Then

Tap [Update] to switch between the fixed end and active end of the caliper. Or

Tap [Clear All] to cancel setting the starting point. Or,

Tap the arrows around the hand icon to fine-tune the cursor position.

4. Tap the hand icon to set the end point.

## 2.2.3 Angle

Function: On B/C image, measures the angle of two crossing planes on the image and the range is:  $0^{\circ}$ - $180^{\circ}$ .

1. Tap [Angle] in the measurement menu.
2. Set two line segments as described in “2.2.2 Distance.”  
The angle appears in the results window after setting the line segments.

## 2.2.4 Area & Circumference

Function: On 2D image, measures the area and circumference of a closed region on the image.  
Four measurement methods are available:

- Ellipse: fix an ellipse region by two equal-cut perpendicular axes.
- Trace: fix a closed region by free tracing.
- Cross: fix a closed region with two axes perpendicular to each other. The starting point and the end point of the axes can both be fixed freely.

### 2.2.4.1 Ellipse

1. Tap [Ellipse] in the measurement menu.
2. Move the cursor to an area of interest.
3. Tap the hand icon to set the starting point of the first axis of the ellipse.
4. Move the cursor to position the end point of the first axis of the ellipse. Then  
Tap [Update] to switch between the fixed end and the active end of the first axis. Or  
Tap [Clear Item] / [Clear All] to clear all calipers.  
Tap the arrows around the hand icon to fine-tune the cursor position.
5. Tap the hand icon to set the end point of the first axis of the ellipse. The second axis appears on the screen.
6. Select and drag the hand icon to increase or decrease the ellipse from the fixed axis and trace the area of interest as closely as possible.  
Tap [Update] to return to the step before setting the first axis. Or,  
Tap [Clear Item] / [Clear All] to clear all calipers. Or,  
Tap the arrows around the hand icon to fine-tune the cursor position.

7. Tap the hand icon to anchor the ellipse region. The measurement result will be displayed in the results window.

### **2.2.4.2 Trace**

1. Tap [Trace] in the measurement menu.
2. Move the cursor to an area of interest.
3. Tap the hand icon to fix the starting point.
4. Move the cursor along the target to trace the outline of the target.  
To modify the line, you can drag the hand icon to move the cursor backward along the trace line.
5. Tap the hand icon and the trace line will be closed with a straight line connecting the start and end points. The trace will also be closed when the cursor is very near to the starting point.

### **2.2.4.3 Cross**

1. Tap [Cross] in the measurement menu.
2. Move the cursor to an area of interest.
3. Tap the hand icon to fix the starting point of the first axis.
4. Position the end point of the first axis and then tap the hand icon. Then tap [Update] to switch between the start point and the end point of the first axis. Or tap [Clear Item] to cancel setting the starting point of the first axis.
5. Tap the hand icon to set the end point of the first axis. The second axis (perpendicular to the first axis) of the cross appears on the screen.
6. Move the cursor and tap the hand icon to fix the starting point of the second axis.
7. Move the cursor to the end point of the second axis. Then tap [Update] to switch between the start point and the end point of the first axis. Or tap [Clear Item] to cancel setting the starting point of the first axis.
8. Tap the hand icon to set the end point of the second axis and fix the region. The results appear in the result window.

## **2.2.5 Curve Length**

Function: measures the length of a curve on the image. Measurement methods available include Trace and Spline.

### **Trace**

1. Select [Trace Len] in the measurement menu. The cursor appears on the screen.
2. Move the cursor to an area of interest.
3. Tap the hand icon to fix the starting point.
4. Move the cursor along the target to trace the outline of the target.  
To modify the line, you can drag the hand icon to move the cursor backward along the trace line.
5. Tap the hand icon to anchor the end point of the trace line.

### **Spline**

1. Select [Trace Len (Spline)] in the measurement menu. The cursor appears on the screen.
2. Move the cursor to an area of interest.

3. Tap the hand icon to fix the starting point.
4. Move the cursor along the target and tap the hand icon to anchor the second, third, fourth, etc., points. A maximum of 12 points can be anchored.  
To correct a previous point, tap [Clear Item].
5. Tap the hand icon twice to set the end point of the spline.

## 2.2.6 Volume

Function: On B/C image, calculates the volume of the target object by the method of 3-distance.

For calculating the object's volume with 3 axes of two images scanned in the plane perpendicular to each other in B mode. The calculation formula is as follows:

$$Volume(cm^3) \square \frac{\pi}{6} \times D1(cm) \times D2(cm) \times D3(cm)$$

Where D1, D2 and D3 are the length of three axes of the target object.

1. Tap [Volume] from the measurement menu.
2. Here D1, D2 and D3 are the lengths of three axes of the target object.  
See "2.2.2 Distance" for detailed procedures.  
Generally D1, D2 and D3 should belong to different scanning planes.

## 2.2.7 Ratio (D)

Function: On 2D/M image, measures the lengths of two line segments and then calculates their ratio.

1. Tap [Ratio (D)] in the measurement menu.
2. Measure the length of the two line segments, see "2.2.2 Distance" for detailed procedures.  
The results display in the results window after the measurement of the second line is completed.

## 2.2.8 Ratio (A)

Function: On 2D image, measures the area of two closed regions and then calculates their ratio. The methods are Ellipse, Trace, Cross and Spline.

1. Tap [Ratio (A)] in the measurement menu.
2. Measure the area of the two closed regions; you may select different measurement methods for each region.

See "2.2.4 Area" for the Ellipse and Trace methods.

### Spline

1. Select [Spline] in the menu.
2. Move the cursor to an area of interest.
3. Tap the hand icon to set the first reference point of the spline.
4. Move the cursor along the area of interest and tap the hand icon to anchor the second reference point.
5. Continue to move and a spline defined by three points of the first and second reference points and the active cursor appears on the screen.

6. Move the cursor along the edge of the target and set more reference points (12 at most) to make the spline approach the target region as closely as possible.
7. Tap the hand icon twice to anchor the last reference point. The spline is fixed and the results display in the results window.

### **Cross**

9. Select [Cross] in the menu.
10. Move the cursor to an area of interest.
11. Tap the hand icon to fix the starting point of the first axis.
12. Move the cursor to position the end point of the first axis and then  
Tap [Update] to switch between the start point and the end point of the first axis. Or,  
Tap [Clear All] to clear all calipers. Or,  
Tap the arrows around the hand icon to fine-tune the cursor position.
13. Tap the hand icon to set the end point of the first axis. The second axis (perpendicular to the first axis) of the cross appears on the screen.
14. Move the cursor and tap the hand icon to fix the starting point of the second axis.
15. Move the cursor to the end point of the second axis. Then  
Tap [Update] to switch between the start point and the end point of the first axis. Or  
Tap [Clear All] to clear all calipers. Or,  
Tap the arrows around the hand icon to fine-tune the cursor position.
16. Tap the hand icon to set the end point of the second axis and fix the region. The results appear in the result window.

## **2.2.9 Smart Trace**

Function: helps the operator to trace the contour of the target by automatically recognizing the margin of the target and measures the lengths of major axis and minor axis, area and circumference of the closed region.

**Tip:** Smart Trace should be performed on frozen images.

1. After the image is frozen, tap [Smart Trace] in the measurement menu.
2. Move the cursor to an area of interest.
3. Tap the hand icon to fix the starting point.
4. Move the cursor along the target to trace the outline of the target.  
During tracing, you can move the cursor backwards to delete latest tracing. Or, you can tap the hand icon to fix the traced contour.  
The faster the cursor moving speed, the bigger the cursor, and the larger the recognized area.
5. Tap the hand icon twice and the trace line will be closed with a straight line connecting the start and end points. The trace will also be closed when the cursor is very near to the starting point.

## **2.2.10 Time**

Function: On M/Doppler image, measures the time interval between two points on the M Mode image.

1. Tap [Time] in the measurement menu.
2. Move the cursor of the dotted lines to the measurement starting point and tap the hand icon.

3. Move the cursor to the measurement end point. The cursor can only be moved in a horizontal direction. Then  
Tap [Update] to switch between the fixed end and active end of the caliper. Or  
Tap [Clear All] to clear all calipers. Or,  
Tap the arrows around the hand icon to fine-tune the cursor position.
4. Tap the hand icon to set the end point.

## 2.2.11 Slope

Function: On M image, measures the distance and time between two points on the M Mode image and calculates the slope between the two points.

1. Tap [Slope] in the measurement menu. Two dotted lines perpendicular to each other appear on the screen.
2. Move the cursor of the dotted lines to the measurement starting point and tap the hand icon.
3. Move the cursor to the measurement end point. The cursor is connected to the starting point by a dashed line. Then  
Tap [Update] to switch between the fixed end and active end of the caliper. Or  
Tap [Clear All] to clear all calipers.
4. Tap the hand icon to set the end point.

## 2.2.12 HR

Function: On M/Doppler image, measures the time interval of n ( $n \leq 8$ ) cardiac cycles on the M Mode image and calculates the heart rate.

The number of cardiac cycles “n” can be preset in the [System] -> [Measure] preset page.

**⚠ CAUTION:** During the measurement, the number of cardiac cycles between the measurement start and end points must be exactly the same as preset ([Preset] -> [System] -> [Measure]). Otherwise, misdiagnosis may occur.

1. Tap [HR] in the measurement menu. The cursor appears in the center of the screen.
2. Select n cardiac cycles.  
The HR result in the results window displays the measured heart rate value and the preset number of cardiac cycles, as shown in the figure below.

HR 76(2) Bpm

Number of Cardiac Cycles

Heart Rate

## 2.2.13 Velocity

Function: On Doppler image, measures the velocity, pressure gradient and correction angle of a certain point on the Doppler spectrum.

1. Tap [Velocity] in the measurement menu.
2. Move the cursor to the point to be measured for velocity.
3. Tap the hand icon to fix it and the result displays in the results window.




## 2.2.14 Acceleration

Function: measures the velocities of two points and their time interval on the Doppler image, and calculates the acceleration, pressure gradient, velocity difference and correction angle.

1. Tap [Acceleration] in the measurement menu.
2. Move the cursor to the first point to be measured for velocity.
3. Tap the hand icon to fix the first point.
4. Move the cursor to the second point to be measured for velocity.
5. Tap the hand icon to fix the second point. The results display in the results window.

## 2.2.15 D Trace

Function: On Doppler image, measures clinical indices using spectral Doppler tracing. Measurement methods available are Trace, Auto, Spline, Vel. (Velocity) and 2 PT (Two Points). A sketch of a Doppler spectrum is shown below:

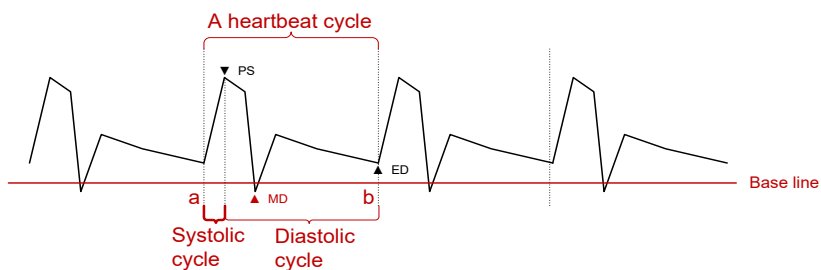

**NOTE:** The heartbeat of the traced spectrum should be equal to that preset, otherwise the obtained HR (Heart Rate) will be incorrect.

- Operations (with the method of Trace):
  1. Tap [D Trace] in the measurement menu.
  2. Move the cursor to the starting point to be measured and tap the hand icon to fix the point.
  3. Drag the hand icon to move the cursor around the object.  
Move the cursor right: draw a trace line overlapping the spectrum as much as possible.  
Move the cursor left to correct the trace line already drawn.
  4. Trace the end point to be measured and tap the hand icon to fix the point.

### Result parameters

The results obtained from D trace are:

Parameters	Descriptions	
PS	Peak Systolic Velocity	The highest velocity of the red blood cells crossing the sample volume.
ED	End-Diastolic Velocity	Measures the blood velocity at the end of the cardiac cycle.

Parameters	Descriptions	
Average velocity	/	<p>The average flow velocity in the whole traced Doppler spectrum.</p> <p>■ TAMAX (Time Averaged Maximum Velocity):</p> $\text{TAMAX}(cm/s) = \frac{\int_{T_a}^{T_b} V(t) dt}{(T_b - T_a)}$ <p>Where V(t) is the maximum velocity</p> <p>■ TAMEAN (Time Averaged Mean Velocity): Obtained by auto-spectrum calculation.</p> $\text{TAMEAN}(cm/s) = \frac{\int_{T_a}^{T_b} V(t) dt}{(T_b - T_a)}$ <p>Where V(t) is the mean velocity.</p>
HR	Heart Rate	Calculates the heart rate per minute by measuring the time interval of one cardiac cycle.
S/D	/	PS/ED. S/D (No unit) = PS (m/s) / ED (m/s)
PI	Pulsatility Index	Pulsatility index. PI (No unit) =  (PS (m/s) – ED (m/s)) / TAMAX (m/s)
RI	Resistive Index	Resistance index. RI (No unit) =  (PS (m/s) – ED (m/s)) / PS (m/s)
θ	/	The correction angle is the spectrum angle during measurement, which is a result obtained from a non D trace measurement tool and is usually displayed together with the spectral measurement results.

**NOTE:**

In the formulae above, T means time, the unit is s; V means the velocity at each point during T, the unit is cm/s; a is the traced starting point, while b is the traced end point.

**Measurement Method**

The measurement method varies according to the result selected.

■ Velocity

Function: measures the velocity and obtain correction angle of a certain point on the Doppler spectrum in the report.

The operations are similar to the Time measurement in M Mode. See “2.2.13 Velocity” for details.

■ 2 PT

Function: measures the velocity, pressure gradient and correction angle between two points on the Doppler spectrum.

1. Select [2 PT] method in the measurement menu.
2. Move the cursor to the starting point to be measured and tap the hand icon to fix the point.
3. Move the cursor to the end point to be measured and tap the hand icon to fix the point.

■ Spline

1. Select [Spline] method from the measurement menu.
2. Move the cursor to the starting point to be measured and tap the hand icon to fix the point.
3. Move the cursor along the edge of the desired region. Continue to fix the second, third, etc., point (50 points at most) of the spectrum.

4. Tap the hand icon twice to anchor the last reference point. Or the measurement ends automatically when there are 50 reference points.

■ Auto

1. Move the cursor to the starting point to be traced and tap the hand icon to fix the point.
2. Move the cursor to the end point of the spectrum to be traced.
3. The system traces the spectrum between the starting and the end point.

■ Auto-Spectrum Calculation

Beside the results listed in table above, you can also obtain results by auto calculation in the following table:

Parameters		Descriptions
MD	Min-Diastolic Velocity	Minimum absolute Velocity in the diastolic cycle.
Vel.	/	Flow velocity
PPG	Peak Pressure Gradient	The corresponding pressure gradient of the peak systolic velocity. $PPG (mmHg) = 4 \times PS (m/s)^2$
Average Pressure Gradient	/	<p>The average pressure gradient in the whole traced Doppler spectrum.</p> <p>■ MPG: Maximum Pressure Gradient.</p> $MPG(mmHg) = \int_{T_a}^{T_b} 4(V(t))^2 dt / (T_b - T_a)$ <p>Where V(t) is the peak systolic velocity.</p> <p>■ MMPG: Mean velocity Mean Pressure Gradient. (Obtained during auto-spectrum calculation.)</p> $MMPG(mmHg) = \int_{T_a}^{T_b} 4(V(t))^2 dt / (T_b - T_a)$ <p>■ Where V(t) is the mean systolic velocity.</p>
VTI	Velocity-Time Integral	<p>Velocity-time integral. The integral of the product of Doppler instantaneous velocity and the total time interval.</p> $VTI(m) = \int_{T_a}^{T_b} V(t) dt$
AT	Acceleration Time	The time of the blood velocity accelerating from the end of diastole to the systolic peak. This is usually the time interval between the end of the first cardiac cycle and the peak of the next cardiac cycle. Choose the first peak when two peaks exist in the systolic cycle.
DT	Deceleration Time	Deceleration Time.
D/S	/	ED/PS. D/S (No unit) = ED (m/s) / PS (m/s)
PV	Peak Velocity	The peak velocity in systolic or diastolic cycles (with no difference), which is the highest velocity of the red blood cells that cross the sample volume. It can be used to examine the venous vessel.

Parameters	Descriptions
------------	--------------

NOTE:

In the formulae above, T means time, the unit is s; V means the velocity at each point during T, the unit is cm/s; a is the traced starting point, while b is the traced end point.

- Tap [Auto Calc.] in the PW image menu to activate it. The system traces automatically and displays the results on the screen.
- Tap [Auto Calc Param] in the [Auto Calc] tab. You can select the parameters to be calculated and displayed.
- Tap [Auto Cardiac Cycle] in the [Auto Calc] image menu. You can select the cycle number to be calculated.

## 2.2.16 D Trace (Car)

Function: On Cardiology Doppler image, measures clinical indices using spectral Doppler tracing. Measurement methods available are Auto, Spline, Vel. (Velocity) and 2 PT (Two Points).

See “3.13 D Trace” for the measurement operations.

### ■ Results

- Vmax
- PGmax
- Vmean
- PGmean
- VTI
- $\theta$  (correction angle)

## 2.2.17 PS/ED

Function: On Doppler image, measures the Peak Systolic (PS) velocity and End Diastolic (ED) velocity on the Doppler spectrum, and calculates their resistance index (RI), S/D and correction angle.

1. Tap [PS/ED] in the measurement menu.
2. Move the cursor to the Systolic Peak and tap the hand icon to fix the point.
3. Move the cursor to the Diastolic End and tap the hand icon to fix the point.

## 2.2.18 Volume Flow

Function: measures blood flow through a vascular cross section per unit time.

1. Tap on [Volume Flow] in the measurement menu.
  - Click [Vas Area] to select the method for calculating the area: dist. or trace.
  - Click [PW Scope] to select the scope to be traced.
2. Measure the vascular area.
3. Click [TAMEAN] or [TAMAX] to calculate the volume flow.

Item	Description	Method or formula
Vas Area	Dist.	Obtain the area by measuring the vascular diameter. $\text{Vas. Area} = \pi \times \text{Vas Diam (cm)}^2 / 4$
	Trace	Obtain the area using the trace method. Area in 2D General Measurements

Item	Description	Method or formula
TAMEAN	Vol Flow(Area) - TAMEAN	$\text{Vol Flow(A) (ml/min)} =  \text{Vas TAMEAN (cm/s)}  \times \text{Vas. Area (cm}^2) \times 60 \text{ (s)}$ Vas. TAMEAN - Time Averaged Mean Velocity, obtained from the Vas. Trace measurement.
TAMAX	Vol Flow(Area) - TAMAX	$\text{Vol Flow(A) (ml/min)} =  \text{Vas TAMAX (cm/s)}  \times \text{Vas Area (cm}^2) \times 60 \text{ (s)}$ Vas. TAMAX - Time Averaged Maximum Velocity, obtained from the Vas. Trace measurement.

## 2.2.19 IMT

**Tip:** The IMT should be performed on frozen images.

IMT (Intima-Media Thickness) measures the distance between LI (Lumen-Intima) and MA (Media-Adventitia). For details, see “6.4.3 Study Tool Operations IMT.”

## 2.3 References

- 3Dist Volume:** Emamian, S.A., et al., "Kidney Dimensions at Sonography: Correlation With Age, Sex, and Habitus in 665 Adult Volunteers," American Journal of Radiology, January, 1993, 160:83-86.
- HR (M general measurement):** Dorland's Illustrated Medical Dictionary, ed. 27, W. B. Sanders Co., Philadelphia, 1988, p. 1425.
- PG:** Powis, R., Schwartz, R. Practical Doppler Ultrasound for the Clinician. Williams & Wilkins, Baltimore, Maryland, 1991, p. 162.
- PPG:** Yoganathan, Ajit P., et al., "Review of Hydrodynamic Principles for the Cardiologist: Applications to the Study of Blood Flow and Jets by Imaging Techniques," Journal of the American College of Cardiology, 1988, Vol. 12, pp. 1344-1353
- MPG:** Yoganathan, Ajit P., et al., "Review of Hydrodynamic Principles for the Cardiologist: Applications to the Study of Blood Flow and Jets by Imaging Techniques," Journal of the American College of Cardiology, 1988, Vol. 12, pp. 1344-1353
- VTI:** Degroff, C. G. Doppler Echocardiography. Third Edition. Lippincott-Raven, Philadelphia, 1999, p. 102-103
- RI:** Burns, P.N., "The Physical Principles of Doppler and Spectral Analysis," Journal of Clinical Ultrasound, November/December 1987, Vol. 15, No. 9, p. 586
- PI:** Burns, Peter N., "The Physical Principles of Doppler and Spectral Analysis," Journal of Clinical Ultrasound, November/December 1987, Vol. 15, No. 9, p. 585
- S/D:** Ameriso S, et al., "Pulseless Transcranial Doppler Finding in Takayasu's Arteritis," J Clin Ultrasound, September 1990; 18:592-6
- D/S:** Ameriso S, et al., "Pulseless Transcranial Doppler Finding in Takayasu's Arteritis," J Clin Ultrasound, September 1990; 18:592-6

# 3 Abdomen

---

The abdomen measurement tools are applied in but not limited to the following exam modes:

- Adult ABD
- EM ABD
- EM AAA

## 3.1 Abdomen Exam Preparations

Make the following preparations before measuring:

1. Confirm that the current probe is appropriate.
2. Check that the current system date is correct.
3. Switch to the correct exam mode.

## 3.2 Basic Abdomen Measurement Procedures

1. Tap [Patient] and register the patient information.
2. Tap [Measure] and select [Advanced] to enter the Advanced Measurements.
3. Select the measurement tool in the menu to start the measurement.  
See section “3.3 Abdomen Measurement Tools” and steps in “2 Basic Measurement” for measurement methods.
4. Tap [Report] to view the exam report. See “3.5 Abdomen Exam Report” for details.

### 3.3 Abdomen Measurement Tools

**NOTE:** The measurement tools mentioned below are configured in the system. The advanced measurement packages provided in this system are generally different combinations of measurement tools.

Measurement, calculation and study measurement items in 2D and Doppler mode (no M mode measurement items) are listed below:

■ Measurement items

Tools	Descriptions	Methods in Basic Measurement	
Liver	/	Distance	
CBD	Common bile duct		
CHD	Common hepatic duct		
GB L	Gallbladder Length		
GB H	Gallbladder Height		
GB wall th.	Gallbladder wall thickness		
Prox Aorta Diam	Prox Abdominal Aorta Diameter		
Mid Sup Aorta Diam	Mid Suprarenal Abdominal Aorta Diameter		
Mid Inf Aorta Diam	Mid Infrarenal Abdominal Aorta Diameter		
Distal Aorta Diam	Distal Abdominal Aorta Diameter		
Aorta Bif Diam	Aorta Bifurcate Diameter		
Iliac Diam	Iliac Diameter		
Ureter	Ureter Diameter		
Pleural L	Pleural Length		
Pleural H	Pleural Height		
Pleural W	Pleural Width		
UQ L	Upper Quadrant Length		
UQ H	Upper Quadrant Height		
UQ W	Upper Quadrant Width		
Pelvis L	Pelvis Length		
Pelvis H	Pelvis Height		
Pelvis W	Pelvis Width		
Pericardial Sac L	Pericardial Sac Length		
Pericardial Sac H	Pericardial Sac Height		
Pericardial Sac W	Pericardial Sac Width		
Prox ABD Aorta	/		D Trace
Mid Sup ABD Aorta	Mid Suprarenal ABD Aorta		



<b>Tools</b>	<b>Descriptions</b>	<b>Methods in Basic Measurement</b>
Mid Inf ABD Aorta	Mid Infrarenal ABD Aorta	
Distal ABD Aorta	/	
IVC	Inferior Vena Cava	Velocity

■ Study items

<b>Tools</b>	<b>Measurement items included</b>	<b>Methods or formulae</b>
Spleen	Spleen L, Spleen H, Spleen W	
Prox Aorta Aneurysm	Prox Aorta Aneurysm L Prox Aorta Aneurysm H Prox Aorta Aneurysm W	
Mid suprarenal Aorta Aneurysm	Mid suprarenal Aorta Aneurysm L Mid suprarenal Aorta Aneurysm H Mid suprarenal Aorta Aneurysm W	
Mid Infrarenal Aorta Aneurysm	Mid Infrarenal Aorta Aneurysm L Mid Infrarenal Aorta Aneurysm H Mid Infrarenal Aorta Aneurysm W	Distance
Distal Aorta Aneurysm	Distal Aorta Aneurysm L Distal Aorta Aneurysm H Distal Aorta Aneurysm W	
Aorta Bif Aneurysm	Aorta Bif Aneurysm L Aorta Bif Aneurysm H Aorta Bif Aneurysm W	
Lliac Aneurysm	Lliac Aneurysm L Lliac Aneurysm H Lliac Aneurysm W	
Kidney	Renal L, Renal H, Renal W, Cortex	Same as Kidney in 8.4.3
Bladder	Pre-BL L, Pre-BL H, Pre-BL W Post-BL L, Post-BL H, Post-BL W	Same as Bladder in 8.4.3
Pleural	Pleural L, Pleural H, Pleural W	
UQ (Upper Quadrant)	UQ L, UQ H, UQ W	
Pelvis	Pelvis L, Pelvis H, Pelvis W	Use Distance to measure the 3 distances and calculates the Volume.
Pericardial Sac	Pericardial Sac L, Pericardial Sac H, Pericardial Sac W	
Smart Bladder	/	See below

## 3.4 Abdomen Measurement Operations

<b>Tip:</b>	<ol style="list-style-type: none"><li>1. See the table in “4 Abdomen Measurement Tools” above for measurement tools and methods.</li><li>2. For the definitions of measurement, calculation and study, see “1.4 Measurement, Calculation and Study”.</li></ol>
-------------	--

1. Select the item/tool in the measurement menu.
2. Perform the measurement referring to the methods in the table above.

### Smart Bladder

<b>NOTE:</b>	Smart Bladder must be used with convex-wide probe.
--------------	--

Function: measure the volume of the urine in the bladder.

1. Scan and obtain the transverse section image of the bladder.
2. Tap [Smart Bladder] in the measurement menu.  
Two diameters d1 and d2 (perpendicular to each other by default) are recognized by the system.
3. If the current result is satisfactory, tap [Accept Result] to save the result.  
Or, if the result is not satisfactory, modify the length and the position of the end points of diameters d1 and d2:
  - a. Move the current activated point to the desired position, and tap [Update] to exchange among the ends of the diameters to adjust the other points as required.  
Tap the arrows around the hand icon to fine-tune the cursor position.
  - b. Tap [Accept Result] to save the result.
4. Tap [UnFreeze] to unfreeze the image.
5. Scan and obtain the longitudinal section image of the bladder.
6. Tap [Measure], the diameter d3 is recognized by the system automatically.
7. If the current result is satisfactory, tap [Accept Result] to save the result.  
Or, if the result is not satisfactory, modify the length and the position of the end points of diameter d3:
  - a. Move the current activated point to the desired position, and tap [Update] to exchange among the ends of the diameter to adjust the other point as required.  
Tap the arrows around the hand icon to fine-tune the cursor position.
  - b. Tap [Accept Result] to save the result.The measurement results will be displayed in the results window.

## 3.5 Abdomen Exam Report

During or after a measurement, tap [Report] to browse the report.

For details about report browsing, printing and exporting, etc., see “1.8 Report.”

# 4 Obstetrics

---

Obstetric measurements are used to estimate the GA and EDD and calculate the growth indices, including the EFW.

The obstetric measurement tools are applied in but not limited to the following exam modes:

- OB1
- OB2/3
- EM OB

## 4.1 Obstetric Exam Preparations

Make the following preparations before measuring:

1. Confirm that the current probe is appropriate.
2. Check that the current system date is correct.
3. Switch to the correct exam mode.

**⚠ CAUTION:** Ensure the system date is correct, otherwise the GA and EDD calculated will be wrong.

## 4.2 Basic Measurement Procedures

1. Tap [Patient] and register the patient information.  
The clinical GA is calculated when the corresponding data is entered on this page. See “4.3.1 Clinical GA” for details.
2. Tap [Measure] and select [Advanced] to enter the Advanced Measurements.
3. Select the measurement tool from the menu to start the measurement.  
See the table in “4.4 Obstetric Measurement Tools” below for measurement tools.  
See section “4.5 Obstetric Measurement Operations” and steps in “2 Basic Measurement” for measurement methods.
4. Tap [Report] to view the exam report. See “4.6 Obstetric Exam Report” for details.

## 4.3 GA

### 4.3.1 Clinical GA

The GA (Gestational Age) and EDD (Estimated Delivery Date) are calculated according to clinical parameters.

1. Tap [Patient] and register the patient information.  
The system automatically calculates the GA and EDD after entering the relative information.



GA (LMP)	21w6d
EDD (LMP)	23/04/2015

The calculation methods are listed as follows:

- LMP: enter the LMP, the system will calculate the GA and EDD.
- DOC: enter the DOC, the system will calculate the GA and EDD.
- IVF: after you enter IVF, the system will calculate the GA and EDD.
- PRV: enter the date and GA of the last exam, the system will calculate a new GA and EDD.
- BBT: after you enter BBT, the system will calculate the GA and EDD.
- EDD: enter the EDD, the system will calculate the GA and LMP.

2. The clinical GA is shown at the top of the obstetric report.

**Tip:** The latest EDD and GA calculation is considered as the final value if more than one EDD and GA calculations are valid.

## 4.3.2 Ultrasound GA

The ultrasound GA and ultrasound EDD are calculated according to the parameters obtained in the measurements.

- GA in OB Items
- AUA (Average Ultrasound Age)

### GA in OB Items

The GA in the OB items is calculated from the related GA tables/formulae. It is independent from the clinical GA.

1. You can preset the GA formulae and whether to display the EDD or not in [System] -> [OB].
2. The GA and other measurement values display in the results window after a measurement.  
If the Diagnostic GA exceeds the threshold, an OOR (out of range) displays in the results window and this result is not recorded in the report.
3. The GA of an OB item displays to the right of the item measurements.
4. For result values used to calculate GA (Gestational Age) and EDD (Estimated Date of Delivery), the formula used in this calculation can be selected from [Formula].

### AUA

AUA is the average of the valid GAs that are calculated according to the biparietal diameter (BPD), head circumference (HC), abdomen circumference (AC), femur length (FL), crown rump length (CRL), etc.

1. All valid values of all the above items will be included in the AUA calculation in the system default method.
2. Touch the checkboxes to the right of the related items to select whether to include the item in the AUA calculation or not. The AUA value varies according to the selection.



Tools	Descriptions	Methods in Basic Measurement
Sac Diam1	Gestational Sac Diameter 1	
Sac Diam2	Gestational Sac Diameter 2	
Sac Diam3	Gestational Sac Diameter 3	
AF1	Amniotic Fluid 1	
AF2	Amniotic Fluid 2	
AF3	Amniotic Fluid 3	
AF4	Amniotic Fluid 4	
Cervix L	Cervical Length	Distance, Trace and Spline
UT L	Uterine Length	
Umb A	Umbilical Artery	2PT, Manual, Spline, Auto
UT H	Uterine Height	Distance in 2D Basic Measurements
UT W	Uterine Width	
Endo.	Endometrium Thickness	
UT A	Uterine Artery	2PT, Manual, Spline, Auto
Ovarian A	Ovarian Artery	
Ovarian V	Ovarian Vein	Velocity
FHR	Fetal Heart Rate	Heart Rate
TAD	Abdominal Transversal Diameter	Distance in 2D Basic Measurements
APAD	Anteroposterior Abdominal Diameter	
OFD	Occipital Frontal Diameter	

■ Calculation and study items

Type	Tools	Measurement items	Methods or formulae
Calculation	TCD/AC	TCD and AC	Measures the TCD, and calculates the ratio of TCD/AC
	Mean Sac Diam	Sac Diam1, Sac Diam2, Sac Diam3	Measures three diameters by Distance method and calculates the average value
	EFW	Estimated Fetal Weight 1	EFW is calculated by the default EFW formula, based on multiple measured parameters. The formula can be reselected in the OB report.
	EFW2	Estimated Fetal Weight 2	
Study	AFI	AF1, AF2, AF3, AF4	Measures in Distance method and calculates AFI
	Uterus	UT L, UT H, UT W, Endo	Distance in Basic Measurement
	Ovary	Ovary L, Ovary H, Ovary W	

## 4.5 Obstetric Measurement Operations

Operations of measurement, calculation and study are described using examples.

<b>Tip:</b>	<ol style="list-style-type: none"> <li>1. See the table in “4.4 Obstetric Measurement Tools” above for measurement tools and methods.</li> <li>2. For the definitions of measurement, calculation and study, see “1.4 Measurement, Calculation and Study.”</li> </ol>
-------------	---

### 4.5.1 Measurement Tool Operations

Take the HC measurement as an example.

1. Select the [HC] item/tool in the measurement menu.  
See “Select Measurement Method Online” for details on how to select a method online.
2. Measure the area according to the Area method in 2D Basic Measurements.  
The measurement results and GA calculation display in the results window.  
You can preset whether to display the EDD or not in [Setup] -> [System] -> [OB] -> [Fetal Gestational Age].

For more details about GA, see “4.3 GA.”

### 4.5.2 Calculation Tool Operations

Take the EFW measurement as an example.

1. Select the [EFW] item/tool in the measurement menu.
2. Measure the FL and AC (for example).  
The second measurement is activated automatically when the first one is completed. The results display in the results window after measurement.

### 4.5.3 Study Tool Operations

The operation of the AFI measurement is as follows:

1. Tap [AFI] in the measurement menu. Enter the submenu.
2. Measure the maximum AFs of the four amniotic fluid pockets of pregnant woman. The AFI is calculated automatically.

## 4.6 Obstetric Exam Report

During or after a measurement, t [Report] to browse the report.

For details about report browsing, printing and exporting, etc., see “1.8 Report.”

## 4.6.1 Fetal Biophysical Profile

Fetal Biophysical Profile means to first obtain a few indices related to fetal growth through experiment or measurement and then evaluate the hazardous situation that the fetus is facing by grading these indices respectively.

1. Tap [Checklist] on the OB report page, the fetus Score is listed after the fetal analysis.

The scoring criteria the system provides are based on the Vintzileos formula, as shown in the table below.

Fetal growth index	Score 0	Score 2	Observation time	Remarks
FHR	<2, or Reactive FHR ≤15 bpm	Reactive FHR ≥ 15 bpm, duration ≥ 15s, ≥ 2 times	30 minutes	The score(s) can be manually entered into the system.
FM	≥ 2 fetal movements	FM ≥ 3 times (continuous movement is deemed as 1 time)	30 minutes	
FBM	No FBM or duration ≤ 30s	FBM ≥ 1 times; duration ≥ 30s	30 minutes	
FT	Limbs stretch, no bend, fingers loose	Limbs and spine stretch/bend ≥ 1 times	/	
AF	No AF, or AF volume < 2 × 2 cm	One or more AF volumes ≥ 2 × 2 cm	/	

Fetal scoring results criteria:

Total scores	Growth condition
8-10	Normal, chronic asphyxia risk low
4-6	Chronic asphyxia risk suspicious
0-2	Chronic asphyxia risk high

2. The scores of each index as well as the total score will be appended to the report.

## 4.6.2 Fetal Growth Curve

The fetus growth curve compares the measured data of the fetus with the normal growth curve to judge whether the fetus is in normal growth state. The growth curve data is sourced from the Fetal Growth Table.

1. Enter patient information and obstetric information in [Patient Info] → [OB] dialog box.
2. Perform one or more fetal growth parameter tools.
3. Touch [Growth Curve] on the report touch screen to display the Obstetric Growth Curve dialog box. The dialog box displays the growth curve and the position of the measurement value.



- Two drop-down lists above the curve display the measurement item/tool and the formula of the curve, which can be changed.
  - Click the [Print] checkbox to determine whether to include the growth curve in the printed report or not.
  - The green dotted line indicates the clinical GA on the X-axis.
  - Select the number and layout of the curves from [Trend Layout].
  - Click [Previous] to turn the growth curve pages.
4. Click [Done] to confirm the setting and exit the page.

**Tip:** If the patient ID is blank, the clinical GA is not calculated or the measurement value is not valid, the measurement values will not be displayed on the curve.

## 4.7 Obstetric Formula

The obstetric formulae are used in the GA and EFW calculations.

### GA and FG Formulae

GA will be automatically calculated after the corresponding measurements are completed. The system will recalculate the GA after new measurements are completed.

**Tip:** For more information about the GA and Fetal Growth Curve, see “4 Obstetrics.”

The GA formulae are shown in the table below:

Note: “/” means no formula provided for the item.

Tools	GA	FG
EFW/EFW2	Hadlock Tokyo	Hadlock Hansmann Tokyo Brenner William CFEF_20 Persson
GS	Rempen Tokyo Hansmann China	Rempen Tokyo Hansmann Hellman

Tools	GA	FG
CRL	Hadlock Tokyo Jeanty Nelson Robinson Rempen Hansmann China ASUM RobinsonBMUS Verburg	Hadlock Tokyo Robinson Rempen Hansmann ASUM Medvedev
BPD	Hadlock Tokyo Jeanty Kurtz Hansmann Merz Rempen ChittyOI Osaka China Nicolaidis ASUM Verburg(O-O)	Hadlock Tokyo Jeanty Kurtz Sabbagha Hansmann Merz Rempen ChittyOI Osaka Nicolaidis ASUM CFEF_2000/2006 INTERGROWTH_21st Medvedev Verburg
HC	Hadlock Jeanty Hansmann ChittyPL ChittyDer Nicolaidis ASUM	Hadlock Merz Jeanty Hansmann Nicolaidis ASUM CFEF_2000/2006 INTERGROWTH_21st Chitty Medvedev Verburg

Tools	GA	FG
AC	Hadlock Jeanty Merz Nicolaides ASUM CFEF Hansmann Chitty	Hadlock Jeanty Merz Chitty Nicolaides ASUM CFEF_2000/2006 INTERGROWTH_21st Hansmann Medvedev Verburg
FL	Hadlock Tokyo Jeanty Hohler Merz Hansmann Warda Chitty Osaka China Nicolaides ASUM	Hadlock Tokyo Jeanty Merz Hansmann O'Brien Warda Chitty Osaka Nicolaides ASUM CFEF_2000/2006 INTERGROWTH_21st Medvedev Verburg
OFD	Hansmann Nicolaides ASUM Jeanty	Hansmann Merz Nicolaides ASUM INTERGROWTH_21st Jeanty Medvedev
FTA	OSAKA	OSAKA
APAD	/	Merz
TAD	CFEF_2000	Merz CFEF
THD	Hansmann	Hansmann

Tools	GA	FG
HUM	Jeanty ASUM	Jeanty Merz ASUM Medvedev
TCD	Hill Nicolaides	Hill Goldstein Nicolaides Verburg
Mean Sac Diam	Daya Hellman	/
AFI	/	Moore
FL/HC (Hadlock)	/	Hadlock
HC/AC (Campbell)	/	Cambell
Ut A PI	/	Merz
Ut A RI	/	Merz

### Fetal Weight Formulae

EFW is a calculation item. If all tools required for the EFW formula have been performed, EFW will be obtained automatically. The system will recalculate the EFW after new measurements are completed.

<b>Tip:</b>	Formulae of EFW and EFW2 of GA/FG are different from those on the [Fetal Calc] page ([Setup]->[System Preset]->[OB] page).
	<ul style="list-style-type: none"> <li>■ EFW formulae of GA/FG are used to perform the GA calculation or the Fetal Growth Curve based on EFW.</li> <li>■ EFW formulae on the [Fetal Growth] page are used in the EFW calculation based on certain OB measurement results (e.g., AC).</li> </ul>

The Fetal Weight formulae are shown in the following table:

Formulae	Descriptions	Units	
		EFW	Item
Hadlock (AC, FL)	$EFW = 10^{(1.304 + (0.05281*AC) + (0.1938*FL) - (0.004*AC*FL))}$	g	cm
	SD = 0.154*EFW SD Type = ±2SD	g	g
Hadlock (AC, FL, BPD)	$EFW = 10^{(1.335 - (0.0034*AC*FL) + (0.0316*BPD) + (0.0457*AC) + (0.1623*FL))}$	g	cm
	SD = 0.146*EFW SD Type = ±2SD	g	g
Hadlock (AC, FL, HC)	$EFW = 10^{(1.326 - (0.00326*AC*FL) + (0.0107*HC) + (0.0438*AC) + (0.158*FL))}$	g	cm
	SD = 0.148*EFW SD Type = ±2SD	g	g



Hansmann M, Hackelöer BJ, Staudach A  
*Ultraschalldiagnostik in Geburtshilfe und Gynäkologie* 1985

*Studies on Fetal Growth and Functional Developments*, Takashi Okai,  
Department of Obstetrics and Gynecology, Faculty of Medicine, University of  
Tokyo

China

Written by Zhou Yiongchang & Guo Wanxue  
in Chapter 38 of "Ultrasound Medicine" (3rd edition) Science & Technology  
Literature Press, 1997

## CRL

Rempen A., 1991  
*Arztliche Fragen. Biometrie in der Frühgravidität (i. Trimenon):* 425-430.

Hansmann M., Hackelöer B.J., Staudach A.  
*Ultraschalldiagnostik in Geburtshilfe und Gynäkologie* 1985

Hadlock F.P., et al. *Fetal Crown-Rump Length: Reevaluation of Relation to  
Menstrual  
Age (5-18 weeks) with High-Resolution Real-time US. Radiology* 182:501-  
505.

Jeanty P., Romero R. *Obstetrical Sonography*, p. 56. New York, McGraw-Hill,  
1984.

Nelson L. *Comparison of methods for determining crown-rump measurement  
by realtime ultrasound. J Clin Ultrasound* February 1981; 9:67-70.

Robinson H.P., Fleming J.E. *A critical evaluation of sonar crown rump length  
measurements. Br J Obstetric and Gynaecologic* September 1975; 82:702-  
710.

*Fetal Growth Chart Using the Ultrasonotomographic Technique*  
Keiichi Kurachi, Mineo Aoki  
Department of Obstetrics and Gynecology, Osaka University Medical School  
Revision 3 (September 1983)

*Studies on Fetal Growth and Functional Developments*  
Takashi Okai Department of Obstetrics and Gynecology, Faculty of Medicine,  
University of Tokyo

Pam Loughna<sup>1</sup>, Lyn Chitty, Tony Evans, Trish Chudleigh. *Fetal size and  
dating: charts recommended for clinical obstetric practice. British Medical  
Ultrasound Society. ULTRASOUND* August 2009 Volume 17 Number 3

China

Written by Zhou Yiongchang & Guo Wanxue  
in Chapter 38 of "Ultrasound Medicine" (3rd edition) Science & Technology  
Literature Press, 1997

*Ultrasonic fetal Measurement Standards for an Australian Population, compiled by Susan Campbell Westerway - Faculty of Health Sciences University of Sydney*

<http://www.asum.com.au/open.home.htm> Date: December 2003

B.O. VERBURG, E. A. P. STEEGERS, M. DE RIDDER, R. J.M. SNIJDERS, E. SMITH, A. HOFMAN, H. A. MOLL, V. W. V. JADDOE and J. C. M. WITTEMAN. *New charts for ultrasound dating of pregnancy and assessment of fetal growth: longitudinal data from a population-based cohort study. Ultrasound Obstet Gynecol 2008; 31: 388–396* Published online 17 March 2008 in Wiley InterScience ([www.interscience.wiley.com](http://www.interscience.wiley.com)). DOI:10.1002/uog.5225

#### **BPD**

Merz E., Werner G. & Ilan E. T. "Ultrasound in Gynecology and Obstetrics" *Textbook and Atlas 312, 326-336.* 1991 Georg Thieme Verlag, pp.326~327

Rempen A., 1991 *Arztliche Fragen. Biometrie in der Fruhgraviditat (i. Trimenon): 425-430.*

Hansmann M., Hackelöer B.J., Staudach A. *Ultraschalldiagnostik in Geburtshilfe und Gynäkologie 1985*

Jeanty P., Romero R. "Obstetrical Ultrasound." McGraw-Hill Book Company, 1984, pp. 57-61.

Sabbagha R.E., Hughey M. *Standardization of sonar cephalometry and gestational age. Obstetrics and Gynecology October 1978; 52:402-406.*

Kurtz A.B., Wapner R.J., Kurtz R.J., et al. *Analysis of biparietal diameter as an accurate indicator of gestational age. J Clin Ultrasound 1980;8:319-326.*

*Fetal Growth Chart Using the Ultrasonotomographic Technique, Keiichi Kurachi, Mineo Aoki, Department of Obstetrics and Gynecology, Osaka University Medical School Revision 3 (September 1983)*

*Studies on Fetal Growth and Functional Developments, Takashi Okai, Department of Obstetrics and Gynecology, Faculty of Medicine, University of Tokyo*

Chitty L.S., Altman D.G. *British Journal of Obstetrics and Gynaecology January 1994, Vol.101 P29-135.*

*China*

*Written by Zhou Yiongchang & Guo Wanxue*

*in Chapter 38 of "Ultrasound Medicine" (3rd edition) Science & Technology Literature Press, 1997*

*Altmann D.G.; Chitty L.S. New charts for ultrasound dating of pregnancy Obstetrics and Gynecology Vol. 10: 174-191, 1997*

Hadlock F.P., et al. *Estimating Fetal Age: Computer-Assisted Analysis of Multiple Fetal Growth Parameters. Radiology* 1984;152: 497-501

Hansmann, Hackeloer, Staudach, Wittmann. *Ultrasound Diagnosis in Obstetrics and Gynecology. Springer-Verlag, New York, 1985*

Jeanty P., Cousaert E., Hobbins J.C., Tack B., Bracken M., Cantraine F. *A longitudinal Study of fetal head biometry. American Journal of Perinatology; Volume1; Number 2; January 1984; pages 118-128*

R. J. M. Snijders and K. H. Nicolaides. *Fetal biometry at 14-40 weeks' gestation. Ultrasound Obstet. Gynecol. 4 (1994) 34-48*

Norio Shinozuka, Takashi Okai, Masahiko Mizuno. Issued by Shindan & Tiryō Sya Tokyo University, School of Medicine, OB/GYN dept. *How to interpret OB/GYN ultrasound measurement data. 80. Fetal Measurement Obstetrics & Gynecology Chapter 56 Separate volume; 1989, Oct. 27th Publication*

B.O. VERBURG, E. A. P. STEEGERS, M. DE RIDDER, R. J.M. SNIJDERS, E. SMITH, A. HOFMAN, H. A. MOLL, V. W. V. JADDOE and J. C. M. WITTEMAN. *New charts for ultrasound dating of pregnancy and assessment of fetal growth: longitudinal data from a population-based cohort study. Ultrasound Obstet Gynecol* 2008; 31: 388–396 Published online 17 March 2008 in Wiley InterScience ([www.interscience.wiley.com](http://www.interscience.wiley.com)). DOI:10.1002/uog.5225

HC

Merz E., Werner G. & Ilan E. T., 1991  
*Ultrasound in Gynecology and Obstetrics Textbook and Atlas* 312, 326-336.

Jeanty P., Romero R. *"Obstetrical Ultrasound."* McGraw-Hill Book Company, 1984.

Hadlock F.P., et al. *Estimating Fetal Age: Computer-Assisted Analysis of Multiple Fetal Growth Parameters. Radiology* 1984; 152 (No. 2):499.

Hansmann M., Hackelöer B.J., Staudach A.  
*Ultraschalldiagnostik in Geburtshilfe und Gynäkologie* 1985

Chitty L.S., Altman D.G.

*British Journal of Obstetrics and Gynaecology* January 1994, Vol.101  
P29-135.

Chitty L.S., Altman D.G., Hendesson A., Campell S., *Charts of fetal size: 2 Head measurements, Br J Obstetric Gynecology* 1994, Vol 101, P 35-43.

Altmann D.G.; Chitty L.S. *"New charts for ultrasound dating of pregnancy"*  
*Ultrasound in Obstetrics and Gynecology* Vol. 10: 174-191, 1997

Jeanty P., Cousaert E., Hobbins J.C., Tack B., Bracken M., Cantraine F., *"A longitudinal study of fetal head biometry"* *American Journal of Perinatology;* Volume 1; Number 2; January 1984



*Ultrasonic fetal Measurement Standards for an Australian Population.*  
compiled by Susan Campbell Westerway - Faculty of Health Sciences  
University of Sydney <http://www.asum.com.au/open.home.htm> Date:  
December 2003

R. J. M. Snijders and K. H. Nicolaidis. *Fetal biometry at 14-40 weeks'*  
*gestation. Ultrasound Obstet. Gynecol.* 4 (1994) 34-48

**AC**

Merz E., Werner G. & Ilan E. T., 1991  
*Ultrasound in Gynecology and Obstetrics Textbook and Atlas 312*, Georg  
Thieme Verlag, 326-336.

Hadlock F.P., et al. *Estimating Fetal Age: Computer-Assisted Analysis of  
Multiple Fetal Growth Parameters. Radiology* 1984; 152 (No. 2):499.

Jeanty P., Romero R. *A longitudinal study of fetal abdominal growth,*  
*"Obstetrical Ultrasound."* MacGraw-Hill Book Company, 1984.

Chitty L.S., Altman D.G.

*British Journal of Obstetrics and Gynaecology* January 1994, Vol.101  
P29-135.

*Ultrasonic fetal Measurement Standards for an Australian Population.*  
compiled by Susan Campbell Westerway - Faculty of Health Sciences  
University of Sydney <http://www.asum.com.au/open.home.htm> Date:  
December 2003

Crequat, J., Duyme, M., Brodaty, G. *Biometry 2000. Fetal growth charts by  
the French College of fetal ultrasonography and the Inserm U 155.*  
*Gynecol.Obstet Fertil.*, Vol. 28 No. 2, 2000, pages 435-455

Chitty L.S. Altman D.G. Hendesson A. Campell S. *Charts of fetal size: 3.*  
*Abdominal measurements. Br J Obstetric Gynaecology* 1994, Vol 101, pages  
35-43.

Chitty, L.S., Altman, D.G., Henderson, A., Campbell, S. *Charts of fetal size: 3.*  
*Abdominal measurements Br.J.Obstet. Gynaecol.* Vol. 101 No. 2, 1994, pages  
125-131

Hansmann, Hackeloer, Staudach, Wittmann. *Ultrasound Diagnosis in  
Obstetrics and Gynecology* Springer- Verlag, New York, 1986, p.431.

Jeanty P., Cousaert E., Cantraine F. *Normal Growth of the Abdominal  
Perimeter. American Journal of Perinatology; Volume 1 Number 2; January  
1984;*  
pages 129-135

R. J. M. Snijders and K. H. Nicolaidis. *Fetal biometry at 14-40 weeks'*  
*gestation. Ultrasound Obstet. Gynecol.* 4 (1994) 34-48

**FL**

Merz E., Werner G. & Ilan E. T., 1991  
*Ultrasound in Gynaecology and Obstetrics Textbook and Atlas 312*, 326-336.

Hansmann M., Hackelöer B.J., Staudach A.  
*Ultraschalldiagnostik in Geburtshilfe und Gynäkologie* 1995

Hadlock F.P., et al. *Estimating Fetal Age: Computer-Assisted Analysis of Multiple Fetal Growth Parameters. Radiology* 1984; 152 (No. 2):499.

Warda A. H., Deter R. L. & Rossavik, I. K., 1985.  
*Fetal femur length: a critical re-evaluation of the relationship to menstrual age. Obstetrics and Gynaecology*, 66,69-75.

O'Brien G.D., Queenan J.T. (1981)  
*Growth of the ultrasound femur length during normal pregnancy, American Journal of Obstetrics and Gynecology* 141:833-837.

Jeanty P., Rodesch F., Delbeke D., Dumont J. *Estimation of gestational age from measurements of fetal long bones. Journal of Ultrasound Medicine* February 1984; 3:75-79.

Hohler C., Quetel T. *Fetal femur length: equations for computer calculation of gestational age from ultrasound measurements. American Journal of Obstetrics and Gynecology* June 15, 1982; 143 (No. 4):479-481.

Keiichi Kurachi, Mineo Aoki  
*Department of Obstetrics and Gynecology, Osaka University Medical School*  
Revision 3 (September 1983)

*Studies on Fetal Growth and Functional Developments*  
Takashi Okai *Department of Obstetrics and Gynecology, Faculty of Medicine, University of Tokyo*

Chitty L.S., Altman D.G.  
*British Journal of Obstetrics and Gynaecology* January 1994, Vol.101  
P29-135.

Jeanty P., Coussaert E., Cantraine F., Hobbins J.C., Tack B., Struyven J. "A longitudinal Study of fetal limb growth" *American Journal of Perinatology*; Volume 1; Number 2; January 1984;136-144

Jeanty P., Rodesch F., Delbeke D., Dumont J. "Estimation of Gestational Age from Measurements of Fetal Long Bones" *Journal of Ultrasound Medicine*, 3: 75-79, February, 1984

China

Written by Zhou Yiongchang & Guo Wanxue in Chapter 38 of "Ultrasound Medicine" (3rd edition) Science & Technology Literature Press, 1997

ASUM

*Ultrasonic fetal Measurement Standards for an Australian Population, compiled by Susan Campbell Westerway - Faculty of Health Sciences*

University of Sydney. <http://www.asum.com.au/open/home.htm> Date:  
December 2003  
R. J. M. Snijders and K. H. Nicolaides; Fetal biometry at 14-40 weeks' gestation *Ultrasound Obstet. Gynecol.* 4 (1994) 34-48

- THD** Hansmann M., Hackelöer B.J., Staudach A.  
*Ultraschalldiagnostik in Geburtshilfe und Gynäkologie* 1985
- TCD** Hill LM, et al. Transverse cerebellar diameter in estimating gestational age in the large for gestational age fetus, *Obstet Gynecol* 1990; 75:981-985.
- R. J. M. Snijders and K. H. Nicolaides; Fetal biometry at 14-40 weeks' gestation *Ultrasound Obstet. Gynecol.* 4 (1994) 34-48
- FTA** Fetal Growth Chart Using the Ultrasonotomographic Technique  
Keiichi Kurachi, Mineo Aoki  
Department of Obstetrics and Gynecology, Osaka University Medical School  
Revision 3 (September 1983)
- HUM** Merz E., Werner G. & Ilan E. T., 1991  
*Ultrasound in Gynaecology and Obstetrics Textbook and Atlas* 312, 326-336.
- Jeanty P., Rodesch F., Delbeke D., Dumont J. Estimation of gestational age from measurements of fetal long bones. *Journal of Ultrasound Medicine* February 1984; 3:75-79.
- Jeanty P., Cousaert E., Cantraine F., Hobbins J.C., Tack B., Struyven J. "A longitudinal Study of fetal limb growth" *American Journal of Perinatology*; Volume 1; Number 2; January 1984;136-144
- Ultrasonic fetal Measurement Standards for an Australian Population, compiled by Susan Campbell Westerway - Faculty of Health Sciences University of Sydney. <http://www.asum.com.au/open/home.htm> Date: December 2003*
- Ultrasound GA** Hadlock, *Radiology*, 1984 152:497-501
- TAD** Merz E., Werner G. & Ilan E. T., 1991  
*Ultrasound in Gynaecology and Obstetrics Textbook and Atlas* 312, 326-336.
- APAD** Merz E., Werner G. & Ilan E. T., 1991  
*Ultrasound in Gynecology and Obstetrics Textbook and Atlas* 312, 326-336.
- OFD** Merz E., Werner G. & Ilan E. T., 1991  
*Ultrasound in Gynecology and Obstetrics Textbook and Atlas* 312, 326-336.
- Hansmann M., Hackelöer B.J., Staudach A.  
*Ultraschalldiagnostik in Geburtshilfe und Gynäkologie* 1985
- Jeanty P., Cousaert E., Hobbins J.C., Tack B., Bracken M., Cantraine F., "A

*longitudinal study of fetal head biometry” American Journal of Perinatology; Volume 1; Number 2; January 1984*

*Ultrasonic fetal Measurement Standards for an Australian Population, compiled by Susan Campbell Westerway - Faculty of Health Sciences University of Sydney <http://www.asum.com.au/open.home.htm> Date: December 2003*

*Hansmann, Hackelöer, Staudach, (Wittmann). Ultrasound Diagnosis in Obstetrics and Gynecology. Springer- Verlag, New York, 1986, p.433*

*R. J. M. Snijders and K. H. Nicolaides. Fetal biometry at 14-40 weeks' gestation. Ultrasound Obstet. Gynecol. 4 (1994) 34-48*

### **Estimated Fetal Weight (EFW)**

*Merz E., Werner G. & Ilan E. T., Ultrasound in Gynaecology and Obstetrics. Textbook and Atlas 1991 Georg Thieme Verlag, 308-338*

*Hansmann M., Hackelöer B.J., Staudach A., Ultraschalldiagnostik in Geburtshilfe und Gynäkologie 1995*

*Campbell S., Wilkin D. “Ultrasonic Measurement of Fetal Abdomen Circumference in the Estimation of Fetal Weight.” Br J Obstetrics and Gynaecology September 1975; 82 (No. 9):689-697.*

*Hadlock F.P., Harrist R., et al. Estimation of fetal weight with the use of head, body, and femur measurements - a prospective study. American Journal of Obstetrics and Gynecology February 1, 1985; 151 (No. 3):333-337.*

*Shepard M., Richards V., Berkowitz R., Warsof S., Hobbins J. An Evaluation of Two Equations for Predicting Fetal Weight by Ultrasound. American Journal of Obstetrics and Gynecology January 1982; 142 (No. 1): 47-54.*

*Fetal Growth Chart Using the Ultrasonotomographic Technique, Keiichi Kurachi, Mineo Aoki Department of Obstetrics and Gynecology, Osaka University Medical School Revision 3 (September 1983)*

*Studies on Fetal Growth and Functional Developments, Takashi Okai Department of Obstetrics and Gynecology, Faculty of Medicine, University of Tokyo*

*Brenner W.E., Edelman D.A., Hendricks C.H. A standard of fetal growth for the United States of America. VOL. 91, NO. 6, JUNE 1998*

*Hadlock F.P., Harrist R., Martinez-Poyer J. In utero analysis of fetal growth: A sonographic standard. Radiology 1991;181:129-133*

*Ronald Williams, Robert Creasy, George Cunningham, Warren Hawes, Rank Norris, Michiko Tashiro. Fetal Growth and Perinatal Viability in California. Obstetric & Gynecology Vol. 59, NO. 5, May 1982*

Hansmann, Hackeloer, Staudach, Wittmann. *Ultrasound Diagnosis in Obstetrics and Gynecology*. Springer-Verlag, New York, 1986

Shinozuka N., Okai T., Kohzuma S., Mukubo M., Shih C.T., Maeda T., et al. *Formulas for Fetal Weight Estimation by Ultrasound Measurements based on Neonatal Specific Gravities and Volumes*. *American Journal of Obstetrics and Gynecology* 157: 1140-1145; 1987

### **Fetal Biophysical Profile**

Manning FA. *Dynamic ultrasound-based fetal assessment: the fetal biophysical profile score*. Women's Hospital, Department of Obstetrics and Gynecology, Winnipeg, Manitoba, Canada.

*Dynamic ultrasound-based fetal Assessment: The Fetal Biophysical Profile Score*, *Clinical obstetrics and gynecology*, Manning FA,38:26-44,1995a.

### **AFI**

Thomas R., Moore M.D., Jonathan E., Cayle M.D. *The amniotic fluid index in normal human pregnancy*. *American Journal of Obstetrics and Gynecology* May 1990; 162: 1168-1173.

### **CI**

Hadlock, F., Deter, R., Carpenter, R., Park, D. *Estimating Fetal Age: effect of Head Shape on BPD*. *American Journal of Roentgenology*, 137: 83-85, July 1981

### **FL/AC**

Hadlock F., Deter R., Harrist R., Roecker E., Park S. *A Date-Independent Predictor of Intrauterine Growth Retardation: Femur Length/Abdominal Circumference Ratio* *American Journal of Roentgenology*, 141:979-984, November 1983

### **FL/HC(Hadlock)**

Hadlock,F.P., Harrist,R.B., Shah,Y., Park,S.K. *The femur length/head circumference relation in obstetric sonography*. *J Ultrasound Med* 1984, 3: 439-442 (Fetal Growth)

### **HC/AC(Campbell)**

Campbell S. *Ultrasound Measurement of Fetal Head and Abdomen Circumference Ratio in the Assessment of Growth Retardation*. *Obstetrics and Gynaecology*, Vol 84, 165- 174, March 1977

### **FL/BPD**

Hohler C.W., Quetel, T:A: *Comparison of Ultrasound Femur Length and Biparietal Diameter in Late pregnancy*. *American Journal of Obstetrics and Gynecology*, volume 14, No. 7: 759-762, 1-Dec.-1981

### **Ut A RI/MCA RI**

Kurmanavicius J., Florio I., Wisser J., Hebisch G., Zimmermann R., Muller R. et al. *Reference resistance indices of the umbilical, fetal middle cerebral and uterine arteries at 24-42 weeks of gestation*. *Ultrasound Obstet. Gynecol.* 1997;10:112-20.



# 5 Cardiology

---

The cardiac measurement tools are applied in but not limited to the following exam modes:

- Adult Cardiac
- Cardiac Diff
- LVO
- EM Cardiac
- TEE

## 5.1 Cardiac Exam Preparations

Make the following preparations before measuring:

1. Confirm that the current probe is appropriate.
2. Check that the current system date is correct.
3. Switch to the correct exam mode.

## 5.2 Basic Cardiac Measurement Procedures

1. Tap [Patient] and enter the patient information.
2. Tap [Measure] and select [Advanced] to enter the Advanced Measurement.
3. Select the measurement tool from the menu to start the measurement.  
See the table in “5.3 Cardiac Measurement Tools” for measurement tools.  
See section “5.3 Cardiac Measurement Tools” and steps in “2 Basic Measurement” for measurement methods.
4. Tap [Report] to view the exam report. See “5.5 Cardiac Exam Report” for details.

## 5.3 Cardiac Measurement Tools

The system supports the following cardiac measurements:

**NOTE:** The heartbeat of the traced spectrum in VTI measurement should be equal to that preset, otherwise the obtained HR (Heart Rate) will be incorrect.

■ Measurement items

Tools	Descriptions	Methods in basic measurement
Ao Diam (2D/M)	Aorta Diameter	Distance
LA Diam (2D/M)	Left Atrium Diameter	
ACS (2D/M)	Aortic Valve Cusp Separation	
LVOT Diam	Left Ventricular Outflow Tract Diameter	
RVAWd (2D/M)	Right Ventricular Anterior wall thickness at end-diastole	
RVDd (2D/M)	Right Ventricular Diameter at end-diastole	
IVSd (2D/M)	Interventricular Septal Thickness at end-diastole	
LVIDd(2D/M)	Left Ventricular Internal Diameter at end-diastole	
LVPWd (2D/M)	Left Ventricular Posterior wall thickness at end-diastole	
RVAWs (2D/M)	Right Ventricular Anterior wall thickness at end-systole	
RVDs (2D/M)	Right Ventricular Diameter at end-systole	
IVSs (2D/M)	Interventricular Septal Thickness at end-systole	
LVIDs (2D/M)	Left Ventricular Internal Diameter at end-systole	
LVPWs (2D/M)	Left Ventricular Posterior wall thickness at end-systole	
IVC Diam.(Insp.)	Inferior Vena Cava Inspiration Diameter	The system automatic calculates IVC Depth(Expir M), IVC Depth(Insp M), IVC Diam(Expir M), IVC Diam(Insp M), SVC Depth(Insp), SVC Diam(Insp), SVC Depth(Expir), SVC Diam(Expir), IVC-CI, IVC-DI, SVC-CI, SVC-DI value. *1
IVC Diam.(Expir.)	Inferior Vena Cava Expiration Diameter	
SVC Diam.(Insp.)	Superior Vena Cava Inspiration Diameter	
SVC Diam.(Expir.)	Superior Vena Cava Expiration Diameter	
LV Area(d)	Left Ventricular area at end-diastole	The system automatic calculates FAC value. FAC=((LV Area(d)- LV Area(s))/ LV Area(d))*100%
LV Area(s)	Left Ventricular area at end-systole	
RV Area(d)	Right Ventricular area at end-diastole	The system automatic



Tools	Descriptions	Methods in basic measurement
RV Area(s)	Right Ventricular area at end-systole	calculates RV FAC value. RV FAC=((RV Area(d)- RV Area(s))/ RV Area(d)) *100%
IVC Time	Inferior Vena Cava Time	Time
MV VTI	Mitral Valve Velocity-Time Integral	2PT, Spline, Manual, Auto
MR VTI	Mitral Valve Regurgitation Velocity-Time Integral	
LVOT VTI	Left Ventricular Outflow Tract Velocity-Time Integral	
AV VTI	Aorta Valve Velocity-Time Integral	
AV AccT	Aorta Valve Acceleration Time	Time in Doppler General Measurements
AV DecT	Aorta Valve Deceleration Time	
AR DecT	Aortic Valve Regurgitation Deceleration Time	Velocity
TV VTI	Tricuspid Valve Velocity-Time Integral	2PT, Spline, Manual, Auto
RVOT VTI	Right Ventricular Outflow Tract Velocity-Time Integral	
PV VTI	Pulmonary Valve Velocity-Time Integral	
TV AccT	Tricuspid Valve Acceleration Time	Acceleration in Doppler General Measurements
TV DecT	Tricuspid Valve Deceleration Time	
PV AccT	Pulmonary Valve Acceleration Time	
PV DecT	Pulmonary Valve Deceleration Time	
PR Ved	Pulmonary Valve Regurgitation Velocity at end-Diastole	Velocity
RAP	Right Atrium Pressure	Input (0-50)
HR (2D/M)	Heart Rate	Measure manually or input
LA Area	Left Atrium Area	Trace
RA Area	Right Atrium Area	
MV EPSS (2D/M)	Mitral Valve Distance between E-Wave and the interventricular septum EPSS (end point septal separation) of the Mitral valve(MV) is used to evaluate LV function.	Distance
LVA <sub>d</sub> apical	Left Ventricular Long-axis Area at End-diastole in apical view	S-P Ellipse
LVA <sub>s</sub> apical	Left Ventricular Long-axis Area at end-systole in apical view	
MV E Vel	Mitral Valve E-wave Velocity	Velocity
MV A Vel	Mitral Valve A-wave Velocity	
MV AccT	Mitral Valve Acceleration Time	/

Tools	Descriptions	Methods in basic measurement
MV DecT	Mitral Valve Deceleration Time	/
IVC Vel(Insp)	Inferior Vena Cava Inspiration Maximum Velocity	D Vel. in Doppler General Measurements
IVC Vel(Expir)	Inferior Vena Cava Expiration Maximum Velocity	
IVRT	Mitral Valve Isovolumic Relaxation Time	Time
MAPSE	Mitral Annular Plane Systolic Excursion	Time in M General Measurements
TAPSE	Tricuspid Annular Plane Systolic Excursion	Distance
MV Ea(lateral)	Mitral Valve lateral Early diastolic motion	Measure MV E Vel item to get E/Ea result. D Vel. in Doppler General Measurements *2
MV Ea(medial)	Mitral Valve medial Early diastolic motion	Measure MV E Vel item to get E/Ea result. D Vel. in Doppler General Measurements *3
MV Aa(medial)	Mitral Valve medial Late diastolic motion	D Vel. in Doppler General Measurements
MV Sa(medial)	Mitral Valve medial Systolic motion	
MV Aa(lateral)	Mitral Valve lateral Late diastolic motion	
MV Sa(lateral)	Mitral Valve lateral Systolic motion	
TV E Vel	Tricuspid Valve E-wave Flow Velocity	
TV A Vel	Tricuspid Valve A-wave Flow Velocity	
MV PHT	Mitral Valve Pressure Half Time	Time in Doppler General Measurements
TV PHT	Tricuspid Valve Pressure Half Time	
MV ARa(medial)	Mitral Valve medial Acceleration Rate	Acceleration in Doppler General Measurements
MV DRa(medial)	Mitral Valve medial Deceleration Rate	
MV ARa(lateral)	Mitral Valve lateral Acceleration Rate	
MV DRa(lateral)	Mitral Valve lateral Deceleration Rate	
AutoEF	Automatic measuring of the diastolic and systolic sectional planes	See "Measurement Tool Operations".

\*1 means:

$$IVC-CI = |IVC Diam(Expir M) - IVC Diam(Insp M)| / \text{Max}(IVC Diam(Expir M), IVC Diam(Insp M))$$

$$IVC-DI = |IVC Diam(Expir M) - IVC Diam(Insp M)| / \text{Min}(IVC Diam(Expir M), IVC Diam(Insp M))$$

$$SVC-CI = |SVC Diam(Expir) - SVC Diam(Insp)| / \text{Max}(SVC Diam(Expir), SVC Diam(Insp))$$

$$SVC-DI = |SVC Diam(Expir) - SVC Diam(Insp)| / \text{Min}(SVC Diam(Expir), SVC Diam(Insp))$$

\*2 means:

$$E / Ea(lateral)(Nounit) = \frac{MV E Vel(cm/s)}{Ea(lateral)(cm/s)}$$

\*3 means:

$$E / Ea(medial + lateral)(Nounit) = \frac{MV E Vel(cm/s)}{(Ea(medial)(cm/s) + Ea(lateral)(cm/s))/2}$$

■ Calculation items

Tools	Measurements included	Methods in basic measurement or formulae
LA/Ao(2D)	Left Atrium Diameter	LA Diam. (cm)/Ao. Diam. (cm)
LA/Ao(M)	Aorta Diameter	
MV E/A	Mitral Valve E-Vel. Mitral Valve A-Vel.	MV E Vel. (cm/s)/MV A Vel. (cm/s)
MVA(PHT)	Mitral Valve Orifice Area (PHT)	MVA(PHT) (cm <sup>2</sup> ) = 220 / MV PHT (ms)
TV E/A	Tricuspid Valve E-Vel./A-Vel.	TV E/A=TV E Vel(cm/s)/TV A Vel(cm/s)
TVA(PHT)	Tricuspid Valve Orifice Area (PHT)	TVA(PHT)=220/TV PHT(cm <sup>2</sup> )
IVC-CI	IVC Diam.(Insp.)	*1
IVC-DI	IVC Diam.(Expir.)	*2

\*1 means:

$$|IVC Diam. (Insp.) - IVC Diam. (Expir.)| / \text{Max}(IVC Diam. (Insp.), IVC Diam. (Expir.)) \times 100\%$$

\*2 means:

$$|IVC Diam. (Insp.) - IVC Diam. (Expir.)| / \text{Min}(IVC Diam. (Insp.), IVC Diam. (Expir.)) \times 100\%$$

■ Study items

See section 5.4.3.

## 5.4 Cardiac Measurement Operations

- Tip:**
1. See the table in “5.3 Cardiac Measurement Tools” above for measurement tools and methods.
  2. For the definitions of measurement, calculation and study, see “1.4 Measurement, Calculation and Study.”

### 5.4.1 Measurement Tool Operations

1. Tap the item/tool in the measurement menu.

2. Perform the measurement referring to the methods in the table above.

## AutoEF

**Function:** Measure the diastole and diastole planes automatically.

Tip: Only cardiac exam mode supports this function.

Recommend to connect ECG, capture the cine of standard A2C and A4C planes, and select cardiac cycles which have the clear plane of the cardiac muscle and less interference to perform AutoEF measure.

### ■ Measure items

Item	Description
LVLd (A2C)	Left ventricular long-axis length at end diastole (A2C)
LVAAd (A2C)	Left ventricular long-axis area at end diastole (A2C)
LVLs (A2C)	Left ventricular long-axis length at end systole (A2C)
LVAAs (A2C)	Left ventricular long-axis area at end systole (A2C)
LVLd (A4C)	Left ventricular long-axis length at end diastole (A4C)
LVAAd (A4C)	Left ventricular long-axis area at end diastole (A4C)
LVLs (A4C)	Left ventricular long-axis length at end systole (A4C)
LVAAs (A4C)	Left ventricular long-axis area at end systole (A4C)

### ■ Measurement Result

Item	Description
EDV (A2C/A4C/BP)	End-diastolic Left Ventricular Volume
EDV Index (A2C/A4C/BP)	End-diastolic Left Ventricular Volume Index
ESV (A2C/A4C/BP)	End-systolic Left Ventricular Volume
ESV Index A2C/A4C/BP)	End-systolic Left Ventricular Volume Index
SV (A2C/A4C/BP)	Stroke Volume
SI (A2C/A4C/BP)	SV Index
EF (A2C/A4C/BP)	Ejection Fraction
CO (A2C/A4C/BP)	Cardiac Output
CI (A2C/A4C/BP)	Cardiac output index

### ■ Operation

1. Select the [AutoEF] in the measure menu.
2. In apical two-chamber view, measure the following parameters:  
Left ventricular endocardium at end-diastolic, the EDV(A2C) is obtained automatically.  
Left ventricular endocardium at end-systolic, the ESV(A2C) is obtained automatically.
3. In apical four-chamber view, measure the following parameters:  
Left ventricular endocardium at end-diastolic, the EDV(A4C) is obtained automatically.  
Left ventricular endocardium at end-systolic, the ESV(A4C) is obtained automatically.

4. If the height and weight have already been entered, the SV, EF, SI, EDV Index and ESV Index are calculated. ECG obtains the HR automatically. If ECG is not connected, it should start HR on the menu.
5. Select the HR source: ECG or entered.  
The CO and CI are calculated automatically using the entered height and weight values.

## 5.4.2 Calculation Tool Operations

1. Tap item/tool in the measurement menu.
2. The system calculates and displays the results after the measurement items have been completed.

## 5.4.3 Study Tool Operations

### 5.4.3.1 LV (2D/M)

This studies estimates the Left Ventricular (LV) diastolic and systolic capabilities using a series of clinical indices measured on the B or M image. It includes two studies LV(2D) in 2D mode and LV(M) in mode.

#### ■ Study items

Measurements items		Methods in basic measurement
IVSd (2D/M)	Interventricular Septal Thickness at end-diastole	Distance
LVIDd (2D/M)	Left Ventricular Internal Diameter at end-diastole	
LVPWd (2D/M)	Left Ventricular Posterior wall thickness at end-diastole	
IVSs (2D/M)	Interventricular Septal Thickness at end-systole	
LVIDs (2D/M)	Left Ventricular Internal Diameter at end-systole	
LVPWs (2D/M)	Left Ventricular Posterior Wall Thickness at End Systole	
RVDd (2D/M)	Right Ventricular Diameter at end-diastole	
RVAWd (2D/M)	Right Ventricular Anterior wall thickness at end-diastole	
HR	Hear Rate	HR(2D): Input HR(M): Input or measure The input range should within 0-999.

The system provides an automatic measurement experience by defining the above tools in a sequence: RVAW → RVD → IVS → LVID → LVPW. As those indexes are arranged along the long-axis of the left ventricle, you can simply finish the measurement by clicking only 6 times.

#### ■ Results

Results	Descriptions	Formulae
EDV(Teich)	End-diastolic Left Ventricular Volume	$EDV(Teich)(ml) = \frac{7 \times LVIDd(cm)^3}{2.4 + LVIDd(cm)}$
EDV Index(Teich)	End-diastolic Left Ventricular Volume Index	EDV Index=EDV/BSA
ESV(Teich)	End-systolic Left Ventricular Volume	$ESV(Teich)(ml) = \frac{7 \times LVIDs(cm)^3}{2.4 + LVIDs(cm)}$
ESV Index(Teich)	End-systolic Left Ventricular Volume Index	ESV Index=ESV/BSA
SV(Teich)	Stroke Volume	SV(ml) = EDV(ml)-ESV(ml)
EF(Teich)	Ejection Fraction	EF(No unit) = SV(ml)/EDV(ml)
SI(Teich)	SV Index	SI(No unit) = SV(ml)/ Body Surface Area (m <sup>2</sup> )
CO(Teich)	Cardiac Output	CO(l/min) = SV(ml)×HR(bpm)/1000
CI(Teich)	Cardiac output index	CI(No unit) = CO(l/min)/Body Surface Area (m <sup>2</sup> )

■ Operating Procedures

1. Tap [LV (2D)] in the advanced measurement menu.
2. At end-diastole in 2D or M mode, measure LVIDd.  
The LVIDd and EDV value are obtained.
3. At end-systole in 2D or M mode, measure LVIDs  
The LVIDs and ESV value are obtained.  
The system calculates the SV and EF.
4. Obtain HR (input HR in 2D mode, input or manually measure HR in M mode).  
The CO value is obtained.  
If the height and weight have already been entered, the SI, CI EDV Index and ESV Index are calculated.

### 5.4.3.2 CO (LVOT)

■ Study items

Measurements items		Methods in basic measurement
LVOT Diam.	Left Ventricular Outflow Tract Diameter	Distance
LVOT VTI	Left Ventricular Outflow Tract Velocity-Time Integral	D Trace (2PT, Spline, Manual, Auto)
AV HR	Heart Rate	Measure or input (0-999)

■ Results

Results	Descriptions	Formulae
LVOT Area	Left Ventricular Outflow Tract Area	Get from LVOT Diam measurement
LVOT Vmax	Left Ventricular Outflow Tract Maximum Velocity	Get from LVOT VTI measurement
LVOT SV	Left Ventricular Outflow Tract SV	
LVOT SI	Left Ventricular Outflow Tract SI	
LVOT VTI	Left Ventricular Outflow Tract Velocity-Time Integral	
LVOT PGmax	Left Ventricular Outflow Tract Maximum Pressure Gradient	
LVOT Vmean	Left Ventricular Outflow Tract Average Velocity	
LVOT PGmean	Left Ventricular Outflow Tract Minimum Pressure Gradient	
LVOT CO	Left Ventricular Outflow Tract CO	
LVOT CI	Left Ventricular Outflow Tract CI	

■ Operating Procedures

1. Tap [CO (LVOT)] in the advanced measurement menu.

2. Measure LVOT Diam.

The LVOT Area is then calculated.

3. Measure LVOT VTI

The following values are obtained

LVOT Vmax

LVOT SV

LVOT VTI

LVOT PGmax

LVOT Vmean

LVOT PGmean

4. Input or measure HR manually.

The LVOT CO is obtained.

If the height and weight have already been entered, the LVOT SI and LVOT CI are calculated.

### 5.4.3.3 RVSP

The RVSP measures the right ventricular systolic pressure.

■ Study Items

Tools	Descriptions	Operations
TR Vmax	Tricuspid Valve Regurgitation Maximum Velocity	D Vel. in Doppler Basic Measurements
RAP	Right Atrium Pressure	Input (0-50)

■ Study Results

Except for the values in the upper table, the following results can be obtained in this study:

Tools	Descriptions	Formulae
TR PGmax	Tricuspid Valve Regurgitation Pressure Gradient	$TR\ PG_{max} (mmHg) = 4 \times TR\ V_{max} (m/s)^2$
RVSP	Right Ventricular Systolic Pressure	$RVSP(mmHg) = RAP(mmHg) + 4 \times (TR\ V_{max}(m/s))^2$

■ Operating Procedures

1. Tap [RVSP] in the measurement menu.
2. Measure the TR Vmax in Doppler mode.  
The TR PGmax is calculated.
3. Tap [RAP] and input the value(0-50) and
4. Tap [OK] after inputting RAP.  
RVSP is calculated.

### 5.4.3.4 PAEDP

The PAEDP measures the pulmonary artery end diastolic pressure.

■ Study items

Measurements items		Methods in basic measurement
PR Ved	Pulmonary Valve Regurgitation Velocity at end-Diastole	Velocity
RAP	Right Atrium Pressure	Input (0-50)

■ Results

Except for the values in the upper table, the following results can be obtained in this study:

Results	Descriptions	Formulae
PR PGed	Pulmonary Valve Regurgitation Pressure Gradient at end-Diastole	Get from PR Ved measurement
PAEDP	Pulmonary Pressure at end-Diastole	$PAEDP(mmHg) = RAP(mmHg) + 4 \times (PR\ Ved(m/s))^2$

■ Operating Procedures

See the table above for methods and formulae for the measurement items.

### 5.4.3.5 Simpson

You may select to measure single plane (A2C or A4C) only or both planes (A2C and A4C) to study.

■ Study Items

Tools	Descriptions	Operations
A2Cd	Left ventricular long-axis length at end diastole in A2C view	Simpson measurement (Trace/Spline/Auto)
A2Cs	Left ventricular long-axis length at end systole in A2C view	



Tools	Descriptions	Operations
A4Cd	Left ventricular long-axis length at end diastole in A4C view	
A4Cs	Left ventricular long-axis length at end systole in A4C view	
HR	Heart Rate	Entered directly

■ Study Results

Tools	Descriptions	Formulae
EDV(A2C/A4C)	End-diastolic Left Ventricular Volume (A2C/A4C)	$EDV(ml) = \pi \times \frac{LVLd_{apical}(cm)}{20} \times \sum_{i=1}^{20} r_i^2 (cm)$ <p>LVLd apical: Left Ventricular Long-axis Length at End-diastole in apical view, i.e. the long-axis length obtained in measurement.</p> <p><math>r_i</math>: Radii obtained from diastolic measurement</p>
EDV (BP)	End-diastolic Left Ventricular Volume (BP)	*1
ESV(A2C/A4C)	End-systolic Left Ventricular Volume (A2C/A4C)	$ESV(ml) = \pi \times \frac{LVLs_{apical}(cm)}{20} \times \sum_{i=1}^{20} r_i^2 (cm)$ <p>LVLs apical: Left Ventricular Long-axis Length at End-systole in apical view, i.e. the long-axis length obtained in measurement.</p> <p><math>r_i</math>: Radii obtained from systolic measurement</p>
ESV (BP)	End-systolic Left Ventricular Volume (BP)	*2
EDV Index (A2C/A4C/BP)	End-diastolic Left Ventricular Volume Index (A2C/A4C/BP)	EDV Index=EDV/BSA
ESV Index (A2C/A4C/BP)	End-systolic Left Ventricular Volume Index (A2C/A4C/BP)	ESV Index=ESV/BSA
SV	Stroke Volume	See table in "5.4.3.1 LV (2D/M)"
CO	Cardiac Output	
EF	Ejection Fraction	
SI	SV Index	
CI	CO Index	

\*1 means:

$$EDV(ml) = \pi \times \frac{MAX\{LVLd_{2i}(cm), LVLd_{4i}(cm)\}}{20} \times \sum_{i=1}^{20} (r_{2i}(cm) \times r_{4i}(cm))$$

\*2 means:

$$ESV(ml) = \pi \times \frac{\text{MAX}\{LVLs_{2i}(cm), LVLs_{4i}(cm)\}}{20} \times \sum_{i=1}^{20} (r_{2i}(cm) \times r_{4i}(cm))$$

Calculate the LV volume on the apical 2-chamber view image:

$$EDV2(ml) = \pi \times \frac{LVLd_{2i}(cm)}{20} \times \sum_{i=1}^{20} r_{2i}^2(cm)$$

$$ESV2(ml) = \pi \times \frac{LVLs_{2i}(cm)}{20} \times \sum_{i=1}^{20} r_{2i}^2(cm)$$

Calculate the LV volume on the apical 4-chamber view image:

$$EDV4(ml) = \pi \times \frac{LVLd_{4i}(cm)}{20} \times \sum_{i=1}^{20} r_{4i}^2(cm)$$

$$ESV4(ml) = \pi \times \frac{LVLs_{4i}(cm)}{20} \times \sum_{i=1}^{20} r_{4i}^2(cm)$$

Where

$LVLd_{2i}$  – Left ventricular long-axis length at end diastole at apical two-chamber view, which is the long-axis length obtained by EDV(A2C) measurement

$LVLd_{4i}$  – Left ventricular long-axis length at end diastole at apical four-chamber view, which is the long-axis length obtained by EDV(A4C) measurement

$LVLs_{2i}$  – Left ventricular long-axis length at end systole at apical two-chamber view, which is the long-axis length obtained by ESV(A2C) measurement

$LVLs_{4i}$  – Left ventricular long-axis length at end systole at apical four-chamber view, which is the long-axis length obtained by ESV(A4C) measurement

$r_{2i}$  – Radii obtained by EDV(A2C) or ESV(A2C) at apical two-chamber view

$r_{4i}$  – Radii obtained by EDV(A4C) or ESV(A4C) at apical four-chamber view

### (1) Simpson single plane measurement (measure apical A2C or A4C only)

#### ■ Operating Procedures

1. Select [Simpson] from the menu.
2. Measure the endocardium.

Measure the left ventricular endocardium at end-diastolic and set the long axis, the EDV is obtained.

Measure the left ventricular endocardium at end-systolic and set the long axis, the ESV is obtained.

The system calculates the SV and EF.

If the height and weight have already been entered, the SI, EDV Index and ESV Index are calculated.

3. Enter HR value.

The CO and CI are calculated automatically using the entered height and weight values.

#### ■ Measurement Methods

The endocardium can be measured using trace, spline or auto, tap items on the menu to select the method.

##### ● Trace

Trace the endocardium along the edge of the target area using a method similar to the "Trace" method in basic measurements, then set the long axis.



- Spline


Set reference points (up to 12) along the edge of the endocardium using a method similar to the “Spline” method in basic measurements, then set the long axis.

- Auto

- (1) Set points A and B on the touch screen, where
  - A: Left ventricular interventricular septal and mitral valve junction;
  - B: Left ventricular wall and mitral valve junction;
- (2) After setting A and B, the cursor will be automatically displayed at point D (where is considered as the apical part by system detecting). After point D is set, the long axis (line segment CD) and the line that traces the endocardium are displayed. Where
  - C: Midpoint of A and B.
  - D: Apical part of left ventricle.

You can:

- Adjust the long axis
  - a) Place the cursor on the long axis (which turns yellow), then tap on the touch screen.
  - b) Adjust point D (with point C unchanged) after the cursor changes to .
- Adjust the trace line
  - a) Place the cursor on the trace line (which turns yellow), and tap on the touch screen.
  - b) Place the cursor along the endocardium edge to adjust the line after the cursor changes to .

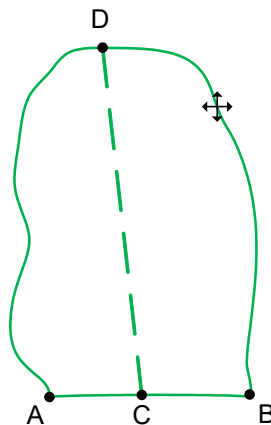

- (3) Tap the hand icon to confirm the adjustment.

## (2) Simpson Bi-plane measurement

**⚠ CAUTION:** When using Simpson to measure LV function, be sure to keep the apical four-chamber view and apical two-chamber view perpendicular. Otherwise the measurement result will be incorrect.

### ■ Operating Procedures

1. Select [Simpson] in the measurement menu.
2. In apical two-chamber view, measure the following parameters:
  - Left ventricular endocardium at end-diastolic and set the long axis, the EDV(A2C) is obtained
  - Left ventricular endocardium at end-systolic and set the long axis, the ESV(A2C) is obtained
3. In apical four-chamber view, measure the following parameters:
  - Left ventricular endocardium at end-diastolic and set the long axis, the EDV(A4C) is obtained
  - Left ventricular endocardium at end-systolic and set the long axis, the ESV(A4C) is obtained

4. If the height and weight have already been entered, the SV, EF, SI, EDV Index and ESV Index are calculated.
5. Enter HR value.

The CO and CI are calculated automatically using the entered height and weight values.

### Mod.Simpson

■ Study Items

Tools	Descriptions	Operations
LVLd apical	Left Ventricular Long-axis Length at End-diastole in apical view	Distance in 2D General Measurements
LVLs apical	Left Ventricular Long-axis Length at End-systole in apical view	
LVAAd sax MV	Left Ventricular Area at Mitral Valve level at End-diastole in Short-axis view	Area in 2D General Measurements
LVAAs sax MV	Left Ventricular Area at Mitral Valve level at End-systole in Short-axis view	
LVAAd sax PM	Left Ventricular Area at Papillary Muscle level at end-diastole in short axis view	
LVAAs sax PM	Left Ventricular Area at Papillary Muscle level at end-systole in short axis view	
HR	Heart Rate	Enter directly

■ Study Results

Tools	Descriptions	Formulae
EDV(Mod.Simpson)	End-diastolic Left Ventricular Volume	*1
ESV(Mod.Simpson)	End-systolic Left Ventricular Volume	*2
EDV Index(Mod.Simpson)	End-diastolic Left Ventricular Volume Index	EDV Index=EDV/BSA
ESV Index(Mod.Simpson)	End-systolic Left Ventricular Volume Index	ESV Index=ESV/BSA
SV(Mod.Simpson)	Stroke Volume	See table in "5.4.3.1 LV (2D/M)"
CO(Mod.Simpson)	Cardiac Output	
EF(Mod.Simpson)	Ejection Fraction	
SI(Mod.Simpson)	SV Index	
CI(Mod.Simpson)	CO Index	

\*1 means:

$$EDV[mL] = \frac{LVLd_{apical} [cm]}{9} \times \left( \frac{4 \times LVA_{dsax} MV [cm^2] + 2 \times LVA_{d sax PM} [cm^2] + \sqrt{LVA_{dsax} MV [cm^2] \times LVA_{dsax PM} [cm^2]}}{sax PM [cm^2] + \sqrt{LVA_{dsax} MV [cm^2] \times LVA_{dsax PM} [cm^2]}} \right)$$

\*2 means:

$$ESV[mL] = \frac{LVLs_{apical} [cm]}{9} \times \left( \frac{4 \times LVA_{ssax} MV [cm^2] + 2 \times LVA_{s sax PM} [cm^2] + \sqrt{LVA_{ssax} MV [cm^2] \times LVA_{ssax PM} [cm^2]}}{sax PM [cm^2] + \sqrt{LVA_{ssax} MV [cm^2] \times LVA_{ssax PM} [cm^2]}} \right)$$

■ Operating Procedures

1. Select [Mod.Simpson] in the measurement menu.
2. In apical long-axis view, measure the following parameters:
  - At end diastole: LVLd apical
  - At end systole: LVLs apical
3. In short-axis view at mitral valve level, measure the following parameters:
  - At end diastole: LVA<sub>d sax MV</sub>
  - At end systole: LVA<sub>s sax MV</sub>
4. In short-axis view at papillary muscle level, measure the following parameters:
  - At end diastole: LVA<sub>d sax PM</sub>, the EDV is calculated
  - At end systole: LVA<sub>s sax PM</sub>, the ESV is calculated

The system calculates the SV and EF.

If the height and weight have already been entered, the SI, EDV Index and ESV Index are calculated.
5. Enter the HR value.
 

The CO and CI are calculated automatically using the entered height and weight values.

## 5.5 Cardiac Exam Report

During or after a measurement, tap [Report] to browse the report.

For details about report browsing, printing and exporting, etc., see “1.8 Report.”

## 5.6 References

Body Surface Area (BSA):

- DuBois, D., DuBois, E.F., “A Formula to Estimate the Approximate Surface Area if Height and Weight Be Known,” *Nutrition*, Sept-Oct 1989, Vol. 5, No. 5, pp. 303-313.

EDV (Teich)

- Folland, E.D., et al., "Assessment of Left Ventricular Ejection Fraction and Volumes by Real-Time, Two-Dimensional Echocardiography," *Circulation*, October 1979, Vol. 60, No.4, pp. 760-766.

ESV (Teich)

- Teichholz, L.E., et al., "Problems in Echocardiographic Volume Determinations: Echocardiographic-Angiographic Correlations in the Presence or Absence of Asynergy," *American Journal of Cardiology*, January 1976, Vol. 37, pp. 7-11. )

Stroke Volume (SV):

- Gorge, G., et al., “High Resolution Two-dimensional Echocardiography Improves the Quantification of Left Ventricular Function,” *Journal of the American Society of Echocardiography*, 1992, 5: 125-34.
- Roelandt, Joseph, *Practical Echocardiology*, vol. 1 of *Ultrasound in Medicine Series*, ed. Denis White, Research Studies Press, 1977, p. 124.

Ejection Fraction (EF):

- Pombo, J.F., “Left Ventricular Volumes and Ejection by Echocardiography,” *Circulation*, 1971, Vol. 43, pp. 480-490.

Stroke Volume Index (SI):

- Gorge, G., et al., “High Resolution Two-dimensional Echocardiography Improves the Quantification of Left Ventricular Function,” *Journal of the American Society of Echocardiography*, 1992, 5: 125-34.
- Roelandt, Joseph, *Practical Echocardiology*, vol. 1 of *Ultrasound in Medicine Series*, ed. Denis White, Research Studies Press, 1977, p. 124.

Cardiac Output (CO):

- Belenkie, Israel, et al., “Assessment of Left Ventricular Dimensions and Function by Echocardiography,” *American Journal of Cardiology*, June 1973, Vol. 31

Cardiac output Index (CI):

- *The Merck Manual of Diagnosis and Therapy*, ed. 15, Robert Berkon, ed., Merck and Co., Rahway, NJ, 1987, p. 378.
- Schiller, N.B., et al., “Recommendations for Quantification of the LV by Two-Dimensional Echocardiography,” *J Am Soc Echo*, Sept.-Oct., 1989, Vol. 2, No. 5,p. 364.

LA/Ao:

- Roelandt, Joseph, Practical Echocardiology, Ultrasound in Medicine Series, Vol. 1, Denis White, ed., Research Studies Press, 1977, p. 270.
- Schiller, N.B., et al., "Recommendations for Quantification of the LV by Two-Dimensional Echocardiography," J Am Soc Echo, Sept-Oct, 1989, Vol. 2, No. 5, p. 364.

MV E/A:

- Maron, Barry J., et al., "Noninvasive Assessment of Left Ventricular Diastolic Function by Pulsed Doppler Echocardiography in Patients with Hypertrophic Cardiomyopathy," Journal of the American College of Cardiology, 1987, Vol. 10, pp. 733-742.

Mitral valve area:

- Goldberg, Barry B., Kurtz, Alfred B., Atlas of Ultrasound Measurements, Year Book Medical Publishers, Inc., 1990, p. 65.
- Stamm, R. Brad, et al., "Quantification of Pressure Gradients Across Stenotic Valves by Doppler Ultrasound," J Am Coll Cardiol, 1983, Vol. 2, No. 4, pp. 707-718.

RVSP(Right Ventricular Systolic Pressure):

- Stevenson, J.G., "Comparison of Several Noninvasive Methods for Estimation of Pulmonary Artery Pressure," Journal of the American Society of Echocardiography, June 1989, Vol. 2, pp. 157-171.
- Yock, Paul G. and Popp, Richard L., "Noninvasive Estimation of Right Ventricular Systolic Pressure by Doppler Ultrasound in Patients with Tricuspid Regurgitation," Circulation, 1984, Vol. 70, No. 4, pp. 657-662.

IVC-CI, IVC-DI

- Fang Junna and Sun Yunbo. "Volume Monitor Indices Review", Chin Crit Care Med, Oct. 2009, Vol. 21, No. 10





# 6 Vascular

---

The vascular measurement tools are applied in but not limited to the following exam modes:

- Vascular
- Carotid
- EM Vascular
- TCI

## 6.1 Vascular Exam Preparations

Make the following preparations before measuring:

1. Confirm that the current probe is appropriate.
2. Check that the current system date is correct.
3. Switch to the correct exam mode.

## 6.2 Basic Vascular Measurement Procedures

1. Tap [Patient] and enter the patient information.
2. Tap [Measure] and select [Advanced] to enter the Advanced Measurement.
3. Tap measurement tool from the menu to start the measurement.

See the table in “6.3 Vascular Measurement Tools” below for measurement tools.

See section “6.4 Vascular Measurement Operations” and steps in “2 Basic Measurement” for measurement methods.

4. Tap [Report] to view the exam report. See “6.5 Vascular Exam Report” for details.

## 6.3 Vascular Measurement Tools

Vascular measurements are mainly used for carotid, cerebral, upper and lower extremity vessels.

The system supports the following 2D and Doppler vascular measurements.

### ■ Measurement items

Tools	Descriptions	Methods in basic measurement
CCA	Common Carotid Artery	2PT, Manual, Spline, Auto
Bulb	Bulbillate	
ICA	Internal Carotid Artery	
ECA	External Carotid Artery	
Vert. A	Vertebral Artery	
C.Iliac V	Common Iliac Vein	Velocity
Ex.Iliac V	External Iliac Vein	
Saph. V	Great Saphenous Vein	

Tools	Descriptions	Methods in basic measurement
Pop. V	Popliteal Vein	
TP Trunk V	Tibial Peroneal Trunk Vein	
Peroneal V	Peroneal Vein	
P.Tib. V	Posterior Tibial Vein	
A.Tib. V	Anterior Tibial Vein	
IVC	Inferior Vena Cava	
ACA	Anterior Cerebral Artery	2PT, Manual, Spline, Auto
MCA	Middle Cerebral Artery	
PCA	Posterior Cerebral Artery	
AComA	Ant.communicating br.	
PComA	Post.communicating br.	
BA	Basilar Artery	
Ba V	Basilar Vein	Velocity
IIV	Internal Iliac Vein	
CFV	Common Femoral Vein	
SFV	Superficial Femoral Vein	
DFV	Deep Femoral Vein	
CCA IMT	Common Carotid Artery IMT	ROI measurement in IMT
Bulb IMT	Bulbillate IMT	
ICA IMT	Internal Carotid Artery IMT	
ECA IMT	External Carotid Artery IMT	

■ Calculation and Study items

Types	Tools	Descriptions	Methods or formulae
Calculation	Stenosis D	Stenosis Diameter	$\text{Stenosis D (No unit)} = \frac{(\text{Normal Diam. (cm)} - \text{Resid Diam. (cm)})}{\text{Normal Diam. (cm)}} \times 100\%$ $\text{Stenosis D (No unit)} = \frac{ (D1-D2) }{\text{MAX}(D1, D2)} \times 100\%$ <p>Where D1 and D2 refer to the measured vascular diameter, and MAX (D1, D2) represents the larger value of the two.</p>
	Stenosis A	Stenosis Area	$\text{Stenosis A (No unit)} = \frac{ (A1-A2) }{\text{MAX}(A1, A2)} \times 100\%$ <p>Where A1 and A2 refer to the measured vascular area, and MAX (A1, A2) represents the larger value of the two.</p>
	ICA/CCA	/	See below

Types	Tools	Descriptions	Methods or formulae
Study	Stenosis A	/	<p>Stenosis (No unit)  <math>=  (A1-A2)/ \text{MAX}(A1,A2)  * 100\%</math></p> <p>Where A1 and A2 refer to the measured vascular area, and MAX (A1, A2) represents the larger value of the two.            You may select different method for the two area measurement.</p>
	IMT	Intima-Media Thickness	See below

## 6.4 Vascular Measurement Operations

- Tip:**
1. See the table in “6.3 Vascular Measurement Tools” above for measurement tools and methods.
  2. For the definitions of measurement, calculation and study, see “1.4 Measurement, Calculation and Study.”

### 6.4.1 Measurement Tool Operations

1. Tap item/tool in the measurement menu.
2. Perform the measurement referring to the methods in the table above.

### 6.4.2 Calculation Tool Operations

#### Stenosis D

Function: measures the Normal Diam. and Resid. Diam., calculates the Stenosis D.

1. Tap [Stenosis D] in the measurement menu.
2. Use the Distance measurement method in 2D Basic Measurements to measure the Normal(D) and Resid(D).

The Stenosis D is calculated automatically.

#### Stenosis A

Function: measures the Normal Area and Resid. Area, calculates the Stenosis A.

1. Tap [Stenosis A] in the measurement menu.
2. Use the Area measurement method in 2D Basic Measurements to measure the Normal(A) and Resid(A).

The Stenosis A is calculated automatically.

## ICA/CCA

Function: measures the flow velocity ratio between ICA and CCA to calculate the stenosis.

1. Tap [ICA/CCA] in the measurement menu.
2. Measure the PS value of the ICA and CCA using the 2 PT method in D trace, and the system calculates the stenosis.

ICA value adopts the latest value that used in an ICA/CCA calculation.

CCA adopts the distal PS value.

## 6.4.3 Study Tool Operations

1. Tap item/tool in the measurement menu.
2. Perform the measurement referring to the methods in the table above.

### IMT


**NOTE:**


1. The IMT function is unavailable on the product not configured with IMT.
2. The IMT measurement is available on frozen (or history) linear array images only.

Function: IMT (Intima-Media Thickness) measures the distance between LI (Lumen-Intima) and MA (Media-Adventia).

The IMT values at 4 positions: CCA (Common Carotid Artery), ICA (Internal Carotid Artery), ECA (External Carotid Artery) and Bulb (Bulbillate) need to be measured here.

1. Select [IMT] in the measurement menu and enter the IMT measurement.
2. Select the side (Left/Right), angle and vessel wall (Near/Far).
3. Select an item such as [ICC, IMT], and the ROI box displays on the screen.

It appears as  when Near is selected

It appears as  when Far is selected

**Tip** Make sure that you select the correct vessel wall (Near/Far) before the IMT measurement. Otherwise the intima may be recognized incorrectly due to different algorithms that are applied in near/far wall recognition.

4. Move the ROI box to the desired position, then tap the hand icon. Two auto trace lines appear in the box.

While the ROI box is green, you can:

- Trace manually
    - a) Drag the hand icon to move the cursor to a target trace line. The trace line turns yellow. Tap the hand icon to confirm.
    - b) Tap along the interface of the vessel. Tap the hand icon to confirm the trace after re-adjusting.
  - Tap [Clear All] to clear all measurement calipers on the screen.
5. Tap the hand icon to confirm the adjustment result after the manual trace is complete. The results are recorded in the IMT report.

The system calculates:

- IMT Max.
- IMT Min.
- IMT Mean

- IMT SD
- IMT ROI Length
- IMT Measure Length
- IMT Quality Index

The Quality Index indicates the reliability of one measurement. Manual trace or re-scan of an image with clear endocardium edges is recommended if the Quality Index value is small.

**Tip:** To achieve a good trace result, try to place the ROI box parallel with the vessel and adjust the box size to reduce unwanted interference.

For multiple measurements on the same side, vessel and angle, the system calculates the following parameters in the report:

- Average Mean IMT
- Average Max. IMT
- Standard deviation

It also provides the Composite Mean IMT, which is an overall mean value of all IMT mean values derived from the measured items.

## 6.5 Vascular Exam Report

During or after a measurement, tap [Report] to browse the report.

For details about report browsing, printing and exporting, etc., see “1.8 Report.”

An IMT report is applied to the record results in the hIMT measurements, where selecting patient conditions (smoker/non-smoker, diabetic/not diabetic, etc.) and modifying the result data are available.

## 6.6 References

**Stenosis D:** Honda, Nobuo, et al., “Echo-Doppler Velocimeter in the Diagnosis of Hypertensive Patients: The Renal Artery Doppler Technique,” *Ultrasound in Medicine and Biology*, 1986, Vol. 12(12), pp. 945-952.

**Stenosis A:** Jacobs, Norman M., et al., “Duplex Carotid Sonography: Criteria for Stenosis, Accuracy, and Pitfalls,” *Radiology*, 1985, 154:385-391.



# 7 Gynecology

---

The gynecology measurement tools are applied in but not limited to the following exam modes:

- GYN

## 7.1 Gynecology Exam Preparations

Make the following preparations before measuring:

1. Confirm that the current probe is appropriate.
2. Check that the current system date is correct.
3. Switch to the correct exam mode.

## 7.2 Basic Gynecology Measurement Procedures

1. Tap [Patient], and register the patient information.
2. Tap [Measure] and select [Advanced] to enter the Advanced Measurement.
3. Tap measurement tool from the menu to start the measurement.

See the table in “7.3 Gynecology Measurement Tools” below for measurement tools.

See section “7.4 Gynecology Measurement Operations” and steps in “2 Basic Measurement” for measurement methods.

4. Tap [Report] to view the exam report. See “7.5 Gynecology Exam Report” for details.

## 7.3 Gynecology Measurement Tools

The system supports the following gynecology measurements.

- Measurement items

Tools	Descriptions	Methods in basic measurement
UT H	Uterine Height	Distance
UT W	Uterine Width	
UT L	Uterine Length	Distance, Trace and Spline
Cervix L	Uterine Cervix Length	
Cervix H	Uterine Cervix Height	
Cervix W	Uterine Cervix Width	Distance
Endo	Endometrium Thickness	
Ovary L	Ovary Length	
Ovary H	Ovary Height	
Ovary W	Ovary Width	

Tools	Descriptions	Methods in basic measurement
Follicle1~16 L	Follicle 1~16 Length	
Follicle1~16 W	Follicle 1~16 Width	
Follicle1~16 H	Follicle1~16 Height	
Ovarian A	Ovarian Artery	2PT, Spline, Manual, Auto
Ut A	Uterine Artery	
Ovarian V	Ovarian Vein	Velocity

■ Calculation and Study items

Types	Tools	Descriptions	Methods or formulae
Calculation	Ovary Vol.	Ovary Volume	See below
	UT Vol.	UT Volume	
	Uterus SUM	/	
	UT-L/ CX-L	/	
	Follicle 1-16	/	
Study	Uterus	/	
	Ovary	/	
	Follicle 1~16	/	
	Follicle	/	
	Ovary	/	

## 7.4 Gynecology Measurement Operations

- Tip:**
1. See the table in “7.3 Gynecology Measurement Tools” above for measurement tools and methods.
  2. For the definitions of measurement, calculation and study, see “1.4 Measurement, Calculation and Study.”

### 7.4.1 Measurement Tool Operations

All items are measured using the Distance method except for UT L and Cervix L which support the Distance, Trace and Spline methods.

### 7.4.2 Calculation Tool Operations

#### Ovary Vol.

Function: measures the Ovary L, Ovary H and Ovary W, calculates the Ovary Vol.

NOTE: needs to be measured on the left and right sides respectively.

1. Tap [Ovary Vol.] in the measurement menu.
2. Use the Distance method in 2D Basic Measurements to measure the Ovary L, Ovary H and Ovary W. The Ovary Vol. is calculated automatically.



## UT Vol

Function: measures the UT L, UT H and UT W, calculates the UT Vol.

1. Tap [UT Vol.] in the measurement menu.
2. Use the Distance method in 2D Basic Measurements to measure the UT L, UT H and UT W. The UT Vol. is calculated automatically.

## UT SUM

Function: measures the UT L, UT H and UT W, calculates Uterus SUM.

$$\text{Uterus SUM (cm)} = \text{UT L (cm)} + \text{UT H (cm)} + \text{UT W (cm)}$$

1. Tap [Uterus SUM] in the measurement menu.
2. Use the Distance method in 2D Basic Measurements to measure the UT L, UT H and UT W. The Uterus SUM are calculated automatically.

## UT-L/ CX-L

Function: measures the UT L and Cervix L, calculates the ratio UT-L/CX-L.

$$\text{UT-L/CX-L (No unit)} = \text{UT L (cm)} / \text{Cervix L (cm)}$$

1. Tap [UT-L/CX-L] in the measurement menu.
2. Use the Distance method in 2D Basic Measurements to measure the UT L and Cervix L. The system calculates the UT-L/CX-L.

## 7.4.3 Study Tool Operations

### Uterus

Function: measures the UT L, UT H, UT W and Endo, calculates the UT Vol., UT SUM and UT-L/CX-L.

1. Tap [Uterus] in the measurement menu.
2. Measure the UT L, UT H, UT W and Endo.  
The UT Vol. and UT SUM are calculated automatically.  
If the Cervix L has been measured, the system also calculates the UT-L/CX-L.

### Ovary

Function: measures the Ovary L, Ovary H and Ovary W, calculates the Ovary Vol.

NOTE: needs to be measured on the left and right sides respectively.

1. Tap [Ovary] in the measurement menu.
2. Use the Distance method in 2D Basic Measurements to measure the Ovary L, Ovary H and Ovary W. The Ovary Vol. is calculated automatically.

### Follicle 1~16

Function: measures the length, width and height of the follicle using the Distance method and calculates the length, width and height averages as well as the follicle volume.

Results	Method	Formulae
Average Diameter	2-distance	Average Diam $\square \frac{(\text{Length} + \text{Width})}{2}$
	3-distance	Average Diam $\square \frac{(\text{Length} + \text{Width} + \text{Height})}{3}$
Follicle Volume	1-distance	Vol $\square \frac{\pi}{6} (\text{Length})^3$

Results	Method	Formulae
	2-distance	$Vol \square \frac{\pi}{6} (Length)^2 \times Width$
	3-distance	$Vol \square \frac{\pi}{6} length \times Width \times Height$

Up to 16 follicles can be measured. Specify the follicle serial numbers before measuring a follicle.

NOTE: needs to be measured on the left and right sides respectively.

Take Follicle1 as an example. The measurements of other items are similar.

1. Tap [Follicle1] in the measurement menu.
2. Use the Distance measurement method in 2D Basic Measurements to measure Follicle1 L, Follicle1 W and Follicle1 H.

The system automatically calculates the average value of Follicle1 L, Follicle1 W and Follicle1 H as well as the volume of Follicle1.

The calculation methods of the follicle diameter and volume can be preset via [Setup] -> [System] -> [Measure].

## 7.5 Gynecology Exam Report

During or after a measurement, tap [Report] to browse the report.

For details about report browsing, printing and exporting, etc., see "1.8 Report."

## 7.6 References

**Uterus SUM:** Feng Kui, Sun Yanling, Li Hezhou. Ultrasonic diagnosis of adenomyosis. Journal of Henan Medical University, 1995; 30 (2).

**UT-L/ CX-L:** Ji Jindi, et al. Ultrasonographic study of the intersex problems and the internal genitalia abnormalities. Journal of China medical ultrasound. 1996, Volume 12, No8 P40.

# 8 Urology

---

The urology measurement tools are applied in but not limited to the following exam modes:

- Urology
- Testical

## 8.1 Urology Exam Preparations

Make the following preparations before performing a urology exam:

1. Confirm that the current probe is appropriate.
2. Check that the current system date is correct.
3. Switch to the correct exam mode.

## 8.2 Basic Urology Measurement Procedures

1. Tap [Patient] and register the patient information.
2. Tap [Measure] and select [Advanced] to enter the Advanced Measurements.
3. Tap measurement tool from the menu to start the measurement.

See the table in “8.3 Urology Measurement Tools” below for measurement tools.

See section “8.4 Urology Measurement Operations” and steps in “2 Basic Measurement” for measurement methods.

4. Tap [Report] to view the exam report. See “8.5 Urology Exam Report” for details.

## 8.3 Urology Measurement Tools

### ■ Measurement Items

Tools	Descriptions	Method in basic measurement
Renal L	Renal Length	Distance
Renal H	Renal Height	
Renal W	Renal Width	
Cortex	Renal Cortical Thickness	
Prostate L	Prostate Length	
Prostate H	Prostate Height	
Prostate W	Prostate Width	
Testicular L	Testicular Length	
Testicular H	Testicular Height	
Testicular W	Testicular Width	
Pre-BL L	Pre-void Bladder Length	

Tools	Descriptions	Method in basic measurement
Pre-BL H	Pre-void Bladder Height	
Pre-BL W	Pre-void Bladder Width	
Post-BL L	Post-void Bladder Length	
Post-BL H	Post-void Bladder Height	
Post-BL W	Post-void Bladder Width	
Epididymis L	Epididymis Length	
Epididymis W	Epididymis Width	
Epididymis H	Epididymis Height	
Scrotal Wall Thickness	/	
Testicular A	Testicular Aorta	2PT, Manual, Spline, Auto
Testicular V	Testicular Vein	Velocity
Epididymis A	Epididymis Aorta	2PT, Manual, Spline, Auto
Epididymis V	Epididymis Vein	Velocity

■ Calculation and study items

Types	Tools	Descriptions	Methods or formulae
Calculation	Renal Vol.	Renal Volume	See below
	Prostate Vol.	Prostate Volume	
	Testicular Vol.	Testicular Volume	
	Pre-BL Vol.	Pre-void Bladder Volume	
	Post-BL Vol.	Post-void Bladder Volume	
	Mictur. Vol.	Micturated Volume	
Study	Kidney	/	See below
	Prostate	/	
	Testis	/	
	Bladder	/	
	Epididymis	/	
	Smart Bladder	/	See Smart Bladder in “3.4 Abdomen Measurement Operations”

## 8.4 Urology Measurement Operations

- Tip:**
1. See the table in “8.3 Urology Measurement Tools” above for measurement tools and methods.
  2. For the definitions of measurement, calculation and study, see “1.4 Measurement, Calculation and Study.”

## 8.4.1 Measurement Tool Operations

All Urology measurement tool operations are the same as the Distance measurement of 2D Basic Measurements.

The measurement procedures are as follows, taking the Prostate L measurement as an example:

1. Tap [Prostate L] in the measurement menu.
2. Use the Distance tool in 2D Basic Measurements to measure the Prostate L.

## 8.4.2 Calculation Tool Operations

### Renal Vol.

Function: measures the Renal L, Renal H and Renal W, calculates the Renal Vol.

NOTE: needs to be measured on the left and right sides respectively.

1. Tap [Renal Vol] in the measurement menu.
2. Use the Distance measurement method in 2D Basic Measurements to measure the Renal L, Renal H and Renal W. The Renal Vol. is calculated automatically.

### Prostate Vol.

Function: measures the Prostate L, Prostate H and Prostate W, calculates the Prostate Vol. and PPSA. If [Serum PSA] in [Patient Info] -> [URO] has been entered, PSAD (Prostate Special Antigen Density) will also be calculated.

$$\text{PPSA (ng/ml)} = \text{PPSA Coefficient (ng/ml}^2\text{)} \times \text{Prostate Vol (ml)}$$

$$\text{PSAD (ng/ml}^2\text{)} = \text{Serum PSA (ng/ml)} / \text{Prostate Vol. (ml)}$$

Here, the PPSA Coefficient and Serum PSA are entered in the [Patient Info] → [URO] dialog box. The default value of the PPSA Coefficient is 0.12.

1. Tap [Prostate Vol.] in the measurement menu.
2. Use the Distance method in Basic Measurements to measure the Prostate L, Prostate H and Prostate W.

The system calculates the Prostate Vol. and PPSA.

The PSAD displays if the PSA value is entered.

### Testicular Vol.

Function: measures the Testis L, Testis H and Testis W, calculates the Testis Vol.

NOTE: needs to be measured on the left and right sides respectively.

1. Tap [Testicular Vol.] in the measurement menu.
2. Use the Distance measurement method in Basic Measurements to measure the Testis L, Testis H and Testis W. The Testis Vol. is calculated automatically.

### Pre-BL Vol.

Function: measures the Pre-BL L, Pre-BL H and Pre-BL W, calculates the Pre-BL Vol.

1. Tap [Pre-BL Vol] in the measurement menu.
2. Use the Distance method in Basic Measurements to measure the Pre-BL L, Pre-BL H and Pre-BL W. The Pre-BL Vol. is calculated automatically. The Mictur.Vol is displayed in the report if the Post-BL Vol is measured.

### **Post-BL Vol.**

Function: measures the Post-BL L, Post-BL H and Post-BL W, calculates the Post-BL Vol.

1. Tap [Post-BL Vol] in the measurement menu.
2. Use the Distance method in Basic Measurements to measure Post-BL L, Post-BL H and Post-BL W. The Post-BL Vol is calculated automatically. The Mictur.Vol is displayed in the report if the Pre-BL Vol is measured.

### **Mictur. Vol.**

Function: measures the Pre-BL Vol and Post-BL Vol, calculates the Mictur.Vol.

1. Tap [Mictur.Vol] in the measurement menu.
2. Use the Distance method in 2D Basic Measurements to measure the Pre-BL L, Pre-BL H and Pre-BL W. The Pre-BL Vol. is calculated automatically and displayed in the report.
3. Use the Distance method in 2D Basic Measurements to measure Post-BL L, Post-BL H and Post-BL W. The Post-BL Vol. and Mictur.Vol. are calculated automatically, the Post-BL Vol. is displayed in the report.

## **8.4.3 Study Tool Operations**

### **Kidney**

Function: measures the Renal L, Renal H and Renal W, calculates the Renal Vol.

NOTE: needs to be measured on the left and right sides respectively.

1. Tap [Kidney] in the measurement menu.
2. Use the Distance measurement method in 2D Basic Measurements to measure the Renal L, Renal H and Renal W. The Renal Vol. is calculated automatically.
3. Use the method of Distance measurement of 2D Basic Measurements to measure Cortex.

### **Prostate**

Function: measures the Prostate L, Prostate H and Prostate W, calculates the Prostate Vol. and PPSA. If [Serum PSA] in [Patient Info] → [URO] has been entered, PSAD (Prostate Special Antigen Density) will also be calculated.

$$\text{PPSA (ng/ml)} = \text{PPSA Coefficient (ng/ml}^2\text{)} \times \text{Prostate Vol (ml)}$$

$$\text{PSAD (ng/ml}^2\text{)} = \text{Serum PSA (ng/ml)} / \text{Prostate Vol. (ml)}$$

Here, the PPSA Coefficient and Serum PSA are entered in the [Patient Info] → [URO] dialog box. The default value of the PPSA Coefficient is 0.12.

1. Tap [Prostate] in the measurement menu.
2. Use the Distance method in 2D Basic Measurements to measure the Prostate L, Prostate H and Prostate W.

The system calculates the Prostate Vol. and PPSA.

The PSAD displays in the report if the PSA value is entered.

### **Testis**

Function: measures the Testis L, Testis H and Testis W, calculates the Testis Vol.

NOTE: needs to be measured on the left and right sides respectively.

1. Tap [Testis] in the measurement menu.
2. Use the Distance measurement method in 2D Basic Measurements to measure the Testis L, Testis H and Testis W. The Testis Vol. is calculated automatically.

## **Bladder**

Function: measures the Pre-BL L, Pre-BL H, Pre-BL W, Post-BL L, Post-BL H and Post-BL W, calculates the Pre-BL Vol., Post-BL Vol and Mictur.Vol.

1. Tap [Bladder] in the measurement menu.
2. Use the Distance method in 2D Basic Measurements to measure the Pre-BL L, Pre-BL H and Pre-BL W. The Pre-BL Vol. is calculated automatically.
3. Use the Distance method in 2D Basic Measurements to measure Post-BL L, Post-BL H and Post-BL W. The Post-BL Vol. and Mictur.Vol. are calculated automatically.

## **Epididymis**

Function: measures the Epididymis L, Epididymis H and Epididymis W.

NOTE: needs to be measured on the left and right sides respectively.

1. Tap [Epididymis] in the measurement menu.
2. Use the Distance measurement method in 2D Basic Measurements to measure Epididymis L, Epididymis H and Epididymis W.

# **8.5 Urology Exam Report**

During or after a measurement, tap [Report] to browse the report.

For details about report browsing, printing and exporting, etc., see "1.8 Report."

## **8.6 References**

**PPSA:** Peter J. Littrup M.D., Fed LeE. M.D., Curtis Mettin. P.D. Prostate Cancer Screening: Current Trends and Future Implications. CA-A CANCER JOURNAL FOR CLINICIANS, Jul/Aug 1992, Vol.42, No.4.

**PSAD:** MITCHELL C. BENSON, IHN SEONG, CARL A. OLSSON, J., McMahon, WILLIAM H.COONER. The Use of Prostate Specific Antigen Density to Enhance the Predictive Value of the Intermediate Levels of Serum Prostate Specific Antigen. THE JOURNAL OF UROLOGY, 1992, Vol.147, p817-821





# 9 Small Parts

---

The small parts measurement tools are applied in but not limited to the following exam modes:

- Thyroid
- Breast
- Testicle
- Superficial
- MSK

## 9.1 Small Parts Exam Preparations

Make the following preparations before measuring:

1. Confirm that the current probe is appropriate.
2. Check that the current system date is correct.
3. Switch to the correct exam mode.

## 9.2 Basic Small Parts Measurement Procedures

1. Tap [Patient] and register the patient information.
2. Tap [Measure] and select [Advanced] to enter the Advanced Measurements.
3. Tap measurement tool in the menu to start the measurement.

See the table in “9.3 Small Parts Measurement Tools” below for measurement tools.

See section “9.4 Small Parts Measurement Operations” and steps in “2 Basic Measurement” for measurement methods.

4. Tap [Report] to view the exam report. See “9.5 Small Parts Exam Report” for details.

## 9.3 Small Parts Measurement Tools

The system supports the following small parts measurements.

- Measurement items

Tools	Descriptions	Methods or formulae
Thyroid L	Thyroid Length	Distance
Thyroid H	Thyroid Height	
Thyroid W	Thyroid Width	
Isthmus H	Isthmus height	
Testicular L	Testicular Length	
Testicular H	Testicular Height	
Testicular W	Testicular Width	

Tools	Descriptions	Methods or formulae
Testis L	Testicular Length	
Testis H	Testicular Height	
Testis W	Testicular Width	
Breast Mass1~10 L	Breast Mass Length	
Breast Mass1~10 H	Breast Mass Height	
Breast Mass1~10 W	Breast Mass Width	
Nip.-Mass 1~10 Dist.	Distance between nipple and mass	
Skin-Mass 1~10 Dist.	Distance between skin and mass	
Thyroid Mass1~3 d1	Thyroid Mass diameter	
Thyroid Mass1~3 d2		
Thyroid Mass1~3 d3		
Epididymis L	Epididymis Length	
Epididymis W	Epididymis Width	
Epididymis H	Epididymis Height	
Scrotal Wall	Scrotal Wall Thickness	
Testicular A	Testicular Aorta	D Trace
Testicular V	Testicular Vein	Velocity
Epididymis A	Epididymis Aorta	D Trace
Epididymis V	Epididymis Vein	Velocity

■ Calculation and study items

Types	Tools	Descriptions	Methods or formulae
Calculation	Thyroid Vol.	Thyroid Volume	Thyroid Vol. (cm <sup>3</sup> ) = k × Thyroid L (cm) × Thyroid H (cm) × Thyroid W (cm) Where k= 0.479 or 0.523
	Testicular Vol.	Testicular Volume	See Testicular Vol. in chapter “8.4.2 Calculation Tool Operations”
Study	Thyroid	/	Same formulae as in the Thyroid Vol. calculation
	Testis	/	See Testis in chapter “8.4.3 Study Tool Operations”
	Breast Mass1~10	/	Volume (3 Dist.)
	Thyroid Mass1~3	/	
	Thyroid Cyst1~3	/	
Epididymis	/	See Epididymis in chapter “8.4.3 Study Tool Operations”	

## 9.4 Small Parts Measurement Operations

- |             |   |
|-------------|---|
| <b>Tip:</b> | <ol style="list-style-type: none"><li>1. See table “9.3 Small Parts Measurement Tools” above for measurement tools and methods.</li><li>2. For the definitions of measurement, calculation and study, see “1.4 Measurement, Calculation and Study.”</li></ol> |
|-------------|---|

### 9.4.1 Measurement Tool Operations

Take the measurement “Thyroid L” for example. The measurement procedure is as follows:

1. Tap [Thyroid L] in the measurement menu.
2. Use the Distance tool in 2D Basic Measurements to measure the Thyroid L. The value displays in the results window and exam report.

### 9.4.2 Calculation Tool Operations

#### Thyroid Vol.

Function: measures Thyroid L, Thyroid H and Thyroid W respectively, and calculates Thyroid Vol.

- |             |  |
|-------------|--|
| <b>Tip:</b> | Needs to be measured on the left and right sides respectively. |
|-------------|--|

1. Tap [Thyroid Vol.] in the measurement menu.
2. Use the Distance tool in 2D Basic Measurements to measure the Thyroid L, Thyroid H and Thyroid W.  
Two Thyroid Vols are calculated automatically.

### 9.4.3 Study Tool Operations

#### Thyroid

Function: measures Thyroid L, Thyroid H and Thyroid W respectively, and calculates Thyroid Vol. See “9.3 Small Parts Measurement Tools” for calculation formulae.

- |             |  |
|-------------|--|
| <b>Tip:</b> | Needs to be measured on the left and right sides respectively. |
|-------------|--|

1. Tap [Thyroid] in the measurement menu.
2. Use the Distance tool in 2D Basic Measurements to measure the Thyroid L, Thyroid H and Thyroid W. The Thyroid Vol. is calculated automatically.

#### Mass

Function: measures the Mass L, Mass W and Mass H to calculate the Mass Volume, as well as measuring the Nip.-Mass Dist. and Skin-Mass Dist. Up to 10 masses can be measured.

Taking Mass1 as an example, the procedure is as follows:

1. Tap [Mass1] in the measurement menu.  
When measuring breast masses, select left or right side from the sub-menu.
2. Use the Distance tool in Basic Measurement to measure Mass1 L, Mass1 W and Mass1 H.
3. Use the Distance tool in Basic Measurement to measure the Nip.-Mass Dist. and Skin-Mass Dist.

The measurements and the calculated Mass Volume are recorded in the report.

## Thyroid Cyst

Function: measures the Thyroid Cyst L, Thyroid Cyst H and Thyroid Cyst W to calculate the Thyroid Cyst Volume. Up to 3 cysts can be measured.

Taking Mass1 as an example, the procedure is as follows:

1. Select [Thyroid Cyst 1] in the measurement menu.  
Select left or right side from the sub-menu.
2. Measure Thyroid Cyst L, Thyroid Cyst W and Thyroid Cyst H by Distance method.  
The system calculates the Thyroid Cyst Volume and the values are recorded in the report.

## Testis

The same as "Testis" in "8 Urology."

## Epididymis

The same as "Epididymis" in "8 Urology."

# 9.5 Small Parts Exam Report

During or after a measurement, tap [Report] to browse the report.

For details about report browsing, printing and exporting, etc., see "1.8 Report."

# 9.6 References

**Thyroid Vol:** Volumetrie der Schilddruesenlappn mittels Realtime-Sonographie; J Brunn, U. Block, G. Ruf, et al.; Dtsch.med. Wschr.106 (1981), 1338-1340.)  
**(k= 0.479)**

**Thyroid Vol:** Gomez J.M., Gomea N., et al. Determinants of thyroid volume as measured by ultrasonography in healthy adults randomly selected. Clin Endocrinol(Oxf), 2000;53:629-634)  
**(k=0.523)**

# 10 Pediatrics

---

The HIP (Hip Joint Angle) measurement is used in pediatric Pediatrics. Such measurement provides early diagnosis for infant hip joint dislocation.

## 10.1 Pediatrics Exam Preparations

Make the following preparations before measuring:

1. Confirm that the current probe is appropriate.
2. Check that the current system date is correct.
3. Switch to the correct exam mode.

## 10.2 Basic Pediatrics Measurement Procedures

1. Tap [Patient] and enter the patient information.
2. Tap [Measure] and select [Advanced] to enter the Advanced Measurement.
3. Tap measurement tool from the menu to start the measurement.

See the table in “10.3 Pediatrics Measurement Tools” below for measurement tools.

See section “10.4 HIP Measurement Operations” and steps in “2 Basic Measurement” for measurement methods.

4. Tap [Report] to view the exam report. See “10.5 Pediatrics Exam Report” for details.

## 10.3 Pediatrics Measurement Tools

**NOTE:** The measurement tools mentioned below are configured in the system. The application measurement packages provided in this system are generally different combinations of measurement tools.

### HIP


The HIP calculation assists in assessing the development of the infant hip. In this calculation, three straight lines are superimposed on the image and aligned with the anatomical features. The two angles are calculated and displayed.

The three lines are:

- The baseline (BL), connecting the osseous acetabular convexity to the point where the joint capsule and the perichondrium unite with the ilium.
- The roof line (RL), connecting the lower edge of the ilium to the osseous acetabular convexity.
- The inclination line (IL), connecting the osseous acetabular convexity to the acetabular labrum.

The angles are:

- $\alpha$ : the angle between BL and RL.
- $\beta$ : the angle between BL and IL.

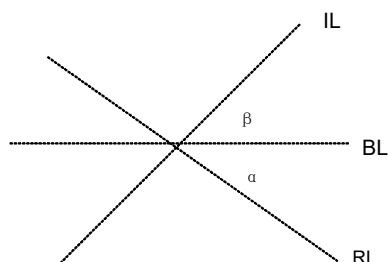

Dislocation type can be determined using the Graf method, as described in the following table.

Type		$\alpha$	Bony roof	Superior bony rim	$\beta$	Cartilaginous roof	Age (Weeks)
I	Ia	$\geq 60^\circ$	good	angular/slightly rounded ("blunt")	$\leq 55^\circ$	covers the femoral head	any age
	Ib	$\geq 60^\circ$	good	angular/slightly rounded ("blunt")	$> 55^\circ$	covers the femoral head	any age
II	IIa	$[50^\circ, 60^\circ)$	adequate (satisfactory)	rounded	any angle	covers the femoral head	$[0, 6]$
	IIa(+)	$[55^\circ, 60^\circ)$	adequate (satisfactory)	rounded	any angle	covers the femoral head	$(6, 12]$
	IIa(-)	$[50^\circ, 55^\circ)$	deficient	rounded	any angle	covers the femoral head	$(6, 12]$
	IIb	$[50^\circ, 60^\circ)$	deficient	rounded	any angle	covers the femoral head	$> 12$


Type		$\alpha$	Bony roof	Superior bony rim	$\beta$	Cartilaginous roof	Age (Weeks)
	IIc	[43°,50°)	severely deficient	rounded to flattened	$\leq 77^\circ$	covers the femoral head	any age
D		[43°,50°)	severely deficient	rounded to flattened	$> 77^\circ$	pressed shift	any age
III	IIIa	$\leq 42^\circ$	poor	flattened	no measure	pressed upwards-without structural alteration (devoid of echoes) proximal perichondrium goes up to the contour of the iliac wall	any age
	IIIb	$\leq 42^\circ$	poor	flattened	no measure	pressed upwards-with structural alteration (they are echogenic) proximal perichondrium goes up to the contour of the iliac wall	any age
IV		$\leq 42^\circ$	poor	flattened	no measure	pressed downwards (horizontal or mulded proximal perichondrium	any age

## HIP-Graf

The measurement items, results and procedures are the same as "HIP."

### d/D

Measures the distance between the baseline and bottom line of the osseous acetabular and the maximum width of the hip to estimate the hip osseous acetabular coverage.

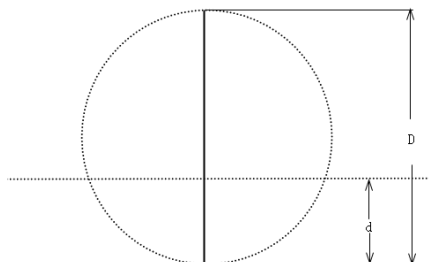

1. Select [d/D] in the measurement menu.
2. The system measures hip width first: Tap to anchor the starting point of the maximum width of the hip (D) and drag the caliper to anchor the end point. A line with a circular fulcrum appears on the measured hip then.
3. Tap and drag the line to determine the relative position of the osseous acetabular so that the distance between the osseous acetabular roof and bottom (d) is measured.
4. The system calculates the d/D.

## 10.4 HIP Measurement Operations

- Tip:**
1. For the definitions of measurement, calculation and study, see “1.4 Measurement, Calculation and Study.”
  2. A measurement tool can be activated by clicking the item in the measurement menu. It is described as “Select/Click ... in the measurement menu” in the following procedures.

1. In B mode, select [HIP] from the measurement menu.  
A line appears, and there is a circular fulcrum on the line.
2. Tap and drag the circle to the position of the hip joint. Then rotate the line to fix the baseline(BL).  
If the image rotates, the baseline will rotate accordingly.
3. Tap the screen outside the circle to confirm and the second line displays.
4. Use the method for adjusting the first line to anchor the roof line (RL) and tap the screen outside the circle to fix the RL.
5. Use the same method to fix the third line inclination line (IL). Angles of  $\alpha$  and  $\beta$  come out.  
If the patient's age is entered, the dislocation type is also displayed.

After the measurement is completed, if the image rotates, the measurement caliper rotates accordingly.

## 10.5 Pediatrics Exam Report

During or after a measurement, tap [Report] to browse the report.

For details about report browsing, printing and exporting, etc., see “1.8 Report.”

## 10.6 References

Graf R., “Sonographic diagnosis of hip dysplasia. Principles, sources of error and consequences” *Ultraschall Med.* 1987 Feb;8(1):2-8

Schuler P., “Principles of sonographic examination of the hip” *Ultraschall Med.* 1987 Feb;8(1):9-1

Graf, R. “Fundamentals of Sonographic Diagnosis of Infant Hip Dysplasia.” *Journal Pediatric Pediatrics*, Vol. 4, No. 6:735-740,1984.

Graf, R. *Guide to Sonography of the Infant Hip.* Georg Thieme Verlag, Stuttgart and New York, 1987.

Morin, C., Harcke, H., MacEwen, G. “The Infant Hip: Real-Time US Assessment of Acetabular Development.” *Radiology*, 177:673-677, December 1985.



# 11 Emergency&Critical

---

The following optional emergency exam modes are available in the current system:

- EM ABD
- EM FAST
- EM OB
- EM Vascular
- EM Superficial
- EM AAA
- EM Cardiac

## 11.1 Basic Measurement Procedures

1. Check the system time, current probe and exam mode are correct.
2. Tap [Patient] and register the patient information.
3. Scan the desired ultrasound views and save the images.
4. Tap [Measure] and select [Advanced] to enter the Advanced Measurements.
5. Tap item/tool to start the measurement.
6. Tap [Report] to view and export the measurement report.

## 11.2 EM Measurement Tools

The commonly used measurement tools are contained in the EM package corresponding to each EM exam mode.

**NOTE:**

1. Measurement tools in each EM package depend on the specific measurement data preset for each ultrasound system.
2. For detailed descriptions of the measurement items, see the corresponding advanced chapter.

## 11.3 EM Exam Report

During or after a measurement, tap [Report] to browse the report.

Each EM exam mode has its corresponding EM report. For details about report browsing, printing and exporting, etc., see “1.8 Report.”



# 12 Nerve

---

## 12.1 Basic Measurement Procedures

1. Check if the system time, current probe and exam mode are correct.
2. Tap [Patient] to register patient information.
3. Scan the desired ultrasonic views and save image(s).
4. Tap [Measure] to enter the measurement menu.
5. Tap item/tool to start the measurement.
6. Tap [Report] to view the measurement report.

## 12.2 Nerve Measurement Tools

There are only basic measurement tools in the Nerve package.

## 12.3 Nerve Exam Report

During or after a measurement, tap [Report] to browse the report.

For details about report browsing, printing and exporting etc, see "1.8 Report".



